

Product Catalog

For Restorative Technologies



Important Product Information For Restorative Products

Instructions For Use:

For detailed information on the specific procedure for the product you are using, please refer to the individual product labels or the appropriate manual on the BIOMET **3i** Website.

Description:

BIOMET **3i** Restorative Products are manufactured from biocompatible titanium, titanium alloy, gold, gold alloy, zirconium, vanadium, stainless steel, polyetheretherketone (PEEK), cobalt chromium alloy, and polyoxymethylene (Delrin). Please refer to product guidelines for use/Surgical Manual for additional device information.

Indications For Use:

BIOMET **3i** Restorative Products are intended for use as accessories to endosseous dental implants for placement in the maxilla and mandible.

Provisional Abutments are intended for use as accessories to endosseous dental implants to support a prosthetic device in a partially or fully edentulous patient. They are intended for use to support a prosthesis in the mandible or maxilla for up to 180 days during endosseous and gingival healing, and are for non-occlusal loading of provisional restorations. The prostheses will either be cement, mechanically or screw-retained to the abutment system based on individual product design. For compatibility of BellaTek® Patient Specific Abutments, please refer to the BellaTek Compatibility Chart (ART 1145).

Contraindications:

Placement of BIOMET **3i** Restorative Products are precluded by known patient hypersensitivity to any of the materials listed in the Description section above.

Warnings:

Mishandling of small components inside the patient's mouth carries a risk of aspiration and/or swallowing. Fracture of a restoration may occur when an abutment is loaded beyond its functional capability. Reuse of BIOMET **3i** Products that are labeled for single-use may result in product contamination, patient infection and/or failure of the device to perform as intended.

PEEK components are intended for use to support single- or multiple-unit provisional prostheses in the mandible or maxilla for up to 180 days, at which time definitive prostheses should be inserted.

Sterility:

Some BIOMET **3i** Restorative Products are supplied sterile. Refer to individual product labels for sterilization information; all sterile products are labeled "STERILE". All products sold sterile are for single-use before the "use by" date printed on the product label. Do not use sterile products if the packaging has been damaged or previously opened. Products provided non-sterile may need to be cleaned and sterilized prior to use. Please refer to the individual product labels or Restorative Manual for more information. For products provided non-sterile

requiring sterilization prior to use, BIOMET **3i** recommends the following sterilization parameters for wrapped items:

Steam gravity sterilization method (gravity-displacement cycle) - Minimum exposure of fifteen (15) minutes timing at a temperature of 270°F (132°C)* **or**

Pre-vacuum sterilization method (dynamic-air-removal cycle) - Minimum exposure of four (4) minutes, four (4) pulses timing at a temperature of 270°F (132°C).*

*Post sterilization, devices should be thoroughly dried for 30 minutes. Please refer to the Surgical and Restorative Manual or package insert for the remaining care and cleaning instructions.

Do not re-sterilize or autoclave components except where indicated on the individual product label, where instructions have been provided in the Restorative Manual or in any additional product literature for the given component.

MRI Statement:

BIOMET **3i** Restorative Products have not been evaluated for safety, heating, migration, or compatibility in the Magnetic Resonance Imaging (MRI) environment.

Precautions:

BIOMET **3i** Restorative Products should only be used by trained professionals. The surgical and restorative techniques required to properly utilize these products are highly specialized and complex procedures. Improper technique can lead to implant failure, loss of supporting bone, restoration fracture, screw loosening and aspiration. Components made from PEEK material are intended for use for up to 180 days.

Potential Adverse Events:

Potential adverse events associated with the use of restorative products may include: failure to integrate; loss of integration; dehiscence requiring bone grafting; infection as reported by: abscess, fistula, suppuration, inflammation, radiolucency; gingival hyperplasia; excessive bone loss requiring intervention; fracture; and nerve injury.

Storage And Handling:

BIOMET **3i** Restorative Products should be stored at room temperature. Refer to the Surgical Manual for special storage or handling conditions.


Caution:

U.S. Federal Law restricts this device to sale by or on the order of a licensed dentist or physician.

Table Of Contents

Introduction

Company Overview	i
Implant & Abutment System Connections	ii
<i>BellaTek</i> ® Patient Specific Technologies Overview	iv
BellaTek® Bars & Frameworks Design Options	v
Restorative Products Flowchart	vii

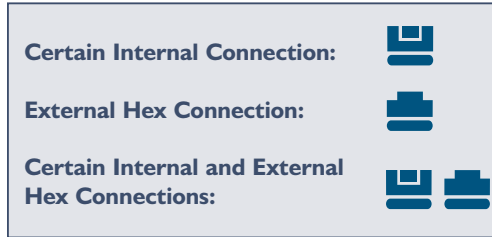

ICON KEY: These icons represent the connection types of the BIOMET **3i** Implant and Abutment Systems for both internal and external connection types represented throughout this catalog.

Restorative Products

Certain® Internal Connection:

Provisional Restorations

PreFormance® Posts	1
PreFormance Temporary Cylinders	2
Titanium Temporary Cylinders	2

Cement-Retained Restorations

GingiHue® Posts	3
ZiReal® Posts	3
GingiHue & ZiReal Post Components	4
UCLA Abutments	5
UCLA Abutment Components	6
Provide® Abutments	7
Provide Abutment Components	8

Screw-Retained Restorations

UCLA Abutments	9
UCLA Abutment Components	10
Low Profile Abutments	11
Low Profile Abutment Components	12

Overdenture Restorations

LOCATOR® Abutments	13
LOCATOR Abutment Components	14

External Hex Connection:

Provisional Restorations

PreFormance Posts	15
PreFormance Temporary Cylinders	16
Titanium Temporary Cylinders	16

Cement-Retained Restorations

GingiHue Posts	17
ZiReal Posts	17
GingiHue & ZiReal Post Components	18
UCLA Abutments	19
UCLA Abutment Components	20

Screw-Retained Restorations

UCLA Abutments	21
UCLA Abutment Components	22
Low Profile Abutments	23
Low Profile Abutment Components	24

Overdenture Restorations

LOCATOR Abutments	25
LOCATOR Abutment Components	26

Continued on next page. ➤

Table Of Contents (Cont'd)

Screws

Certain® Internal Connection:

Abutment, Retaining, Waxing & Try-In Screws 27

External Hex Connection:

Abutment, Retaining, Waxing & Try-In Screws 28

Miscellaneous Restorative Products

Mechanical Driver Kits 29

Drivers & Driver Tips 30

Navigator® System Instrumentation Overview 31

Tapered Navigator Laboratory Kit 32

Parallel Walled Navigator Laboratory Kit 32

Laboratory Tools 33

Miscellaneous Items 33

Patient Education Products 34

Additional Information

Index 35

Ordering Form 42

Ordering Information 44

Introduction

Company Overview



Providing Solutions – One Patient At A Time™

Mission Statement:

BIOMET 3i will be recognized as a global leader in the oral reconstruction marketplace. We will achieve this through superior customer support and continuous product innovation.

Headquartered in Palm Beach Gardens, Florida, with operations throughout the world, BIOMET **3i** is one of the leading companies in the oral reconstruction market. Of equal importance, BIOMET **3i** brings the same innovation, high standards and comprehensive approach to customer service, dental practice and laboratory support and education.

BIOMET **3i** offers one of implant dentistry's most comprehensive lines of implants and abutments, augmented by a growing line of site preparation, digital, restorative and regenerative products.


BIOMET **3i** pioneered the development of biologically driven implants, winning worldwide acclaim for the microtextured OSSEOTITE® surface and then the nano-scaled, Bone Bonding® NanoTite™ Surface Implants. The tradition of implant innovation continues with the introduction of the **3i** T3® Implant, a contemporary hybrid that is designed for sustainable aesthetics.

This spirit of innovation continues with the introduction of DIEM®2, a protocol to enable clinicians to pursue immediate provisionalization options for full arch patient cases.



Introduction


Implant & Abutment System Connections

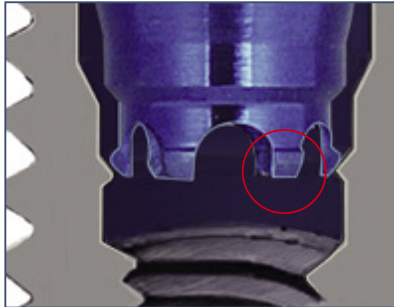


Certain® Internal Connection

The internal connection aspect of the implant and abutment are designed for ease of use and simplicity.

- QuickSeat® Connection: It Clicks! The Certain Implant and Abutment Systems feature the QuickSeat Connection. This unique connection produces an audible and tactile “click” that confirms placement of Impression Copings and Abutments.

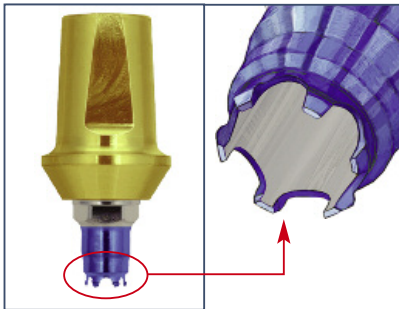



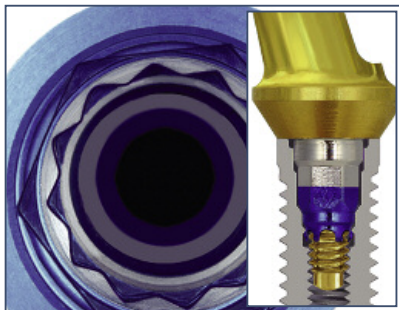

- Abutment fingers cause the “click” and also provide retention for the prosthetic components in the implant before the screw is placed. A screw is needed to fully seat the components when the restoration is being tried in or definitively placed.



- The 6/12 hex inside the internal connection incorporates both a 6-point single and a 12-point double hex. The 6-point single hex has two functions: engaging the driver tip for mountless delivery during implant placement and providing anti-rotation for all straight abutments. The 12-point double hex provides 30° rotational positioning for pre-angled abutments.




- Impression Copings: Pick-Up and Twist Lock™ Transfer Copings are available in the Certain Internal Connection design, in three EP® (Emergence Profile) diameters and a straight diameter to match the corresponding Healing Abutment. The Impression Copings also “click” when properly seated. These copings have a different finger design that engages 2mm internally into the implant, as compared to the abutment’s design that engages 4mm deep into the implant. This shorter engagement into the implant is important because it allows off-axis draw for implant impressions that are divergent.

(purple)	(blue)	(yellow)	(green)
			
3.4mm	4.1mm	5mm	6mm

- Color-Coding: Certain Implants and all interfacing components are color-coded by restorative platform diameter for easy identification and selection.

Introduction


Implant & Abutment System Connections

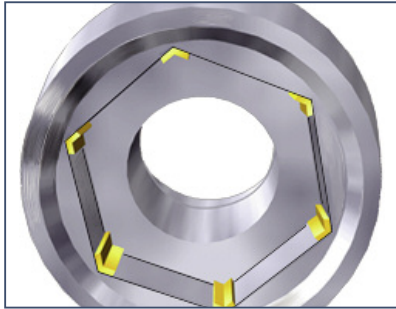


External Hex Connection

The external hex connection implant and abutment designs have been widely used in implant dentistry.


- Gold Standard ZR (Zero Rotation) is a patented design incorporating machined microstops within the corners of the hex in the abutment. The design reduces horizontal rotation between the implant and abutment. Gold Standard ZR is available on UCLA, GingiHue® and Conical Abutments.

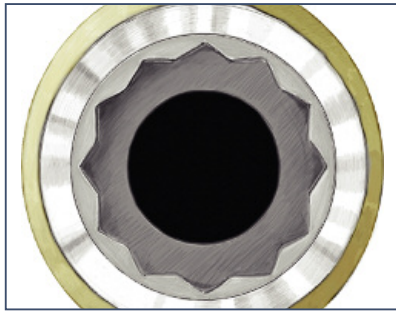

- The 12-point double hex, which is machined in the 15° Pre-Angled GingiHue Abutment, provides rotational positioning in 30° increments on the implant hex.

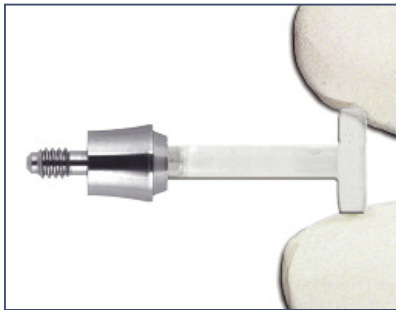

- Precise Abutment Placement: The ASYST Abutment Placement Tool provides fingertip control for fast and easy abutment delivery. The patented packaging design makes abutment placement easier because the abutment is delivered sterile from the package directly to the implant site. The abutment and abutment screw are packaged inside the plastic ASYST seating device. The plastic seating device facilitates precise placement of the abutment on the implant, thus reducing chair time. The ASYST Tool is packaged with Low Profile, Standard and Conical Abutments.

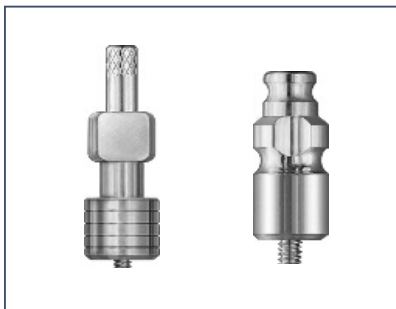

- Impression Copings: Pick-Up and Twist Lock™ Transfer Copings are both available in the external connection design in three EP® (Emergence Profile) diameters and a straight diameter to match the corresponding healing abutment. The patented Twist Lock design provides a more accurate transfer of the implant connection as compared to other transfer (closed tray) techniques. This unique Twist Lock feature provides a series of undercuts to guide the coping into the impression, giving stability to the impression coping/analog prior to pouring the impression. As a result, the copings lock into orientation grooves upon clockwise rotation, thereby allowing for a tactile sensation of resistance that ensures an accurate hex transfer.

Introduction



Patient Specific Technologies Overview



BellaTek® Encode® Impression System

The BellaTek Encode Impression System eliminates the need for an implant-level impression while delivering a patient-specific restoration that has the appropriate margin height and natural emergence contours for the patient. This accuracy is achieved from an impression of the BellaTek Encode Healing Abutment. Codes embedded on the occlusal surface of the BellaTek Encode Healing Abutment communicate the collar height, implant hex-orientation, platform diameter and interface (the Certain® Internal Connection or External Hex Connection) of the implant. Because the tissue is healed at the time of impression, the margin is designed to have the appropriate placement and contour. The result is a patient specific, anatomically designed, final BellaTek Abutment. Available in titanium with or without titanium nitride coating.



BellaTek Bars & Frameworks

BellaTek Bars and Frameworks are created with the technology to achieve a truly passive fit. These are available in Hader and Dolder® Designs for overdenture bars, primary bars and in fixed hybrid designs. This technology does not require any wax or resin design from the technician. The bars can be made on most major dental implants and abutments. Because these are milled from one solid piece of lightweight titanium, the potential for weakness caused by soldering or laser welded joints is eliminated. You receive a completed superstructure ready for prosthesis processing. No polishing or retention creation necessary. **COMET 3** can even tap holes for attachments.

Copymilled Bars are also available for those who prefer to design a bar or framework in a resin pattern to the patient's specifications.










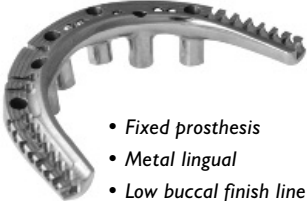


NOTE: Please ensure that as many implants as necessary are used for a fully stable restoration.

Introduction



Bars & Frameworks Design Options

BellaTek® Bars and Frameworks are compatible with all major implant systems and match a wide variety of implant and abutment connections. Please refer to the interface compatibility charts when placing your orders for bars and frameworks with competitive connections. You can also find the BellaTek Bars and Frameworks Design Options and Interface Compatibility Charts by visiting www.bellatek.biomet3i.com.

<p>Hybrid Bar Design #1</p>  <p>• Fixed prosthesis • Metal lingual • Low buccal finish line • Titanium tissue surface</p>		<p>Hybrid Bar Design #2</p>  <p>• Fixed prosthesis • Metal lingual • Low buccal finish line • Titanium tissue surface</p>	
<p>Wraparound Bar</p>  <p>• Fixed prosthesis • Acrylic resin wraparound design • Adjustments possible to accommodate for changing tissue contours • Easy to repair and modify the acrylic resin portion of the prosthesis</p>		<p>Freeform Bar</p>  <p>• Fixed prosthesis • Acrylic resin wraparound design</p>	
<p>Canada Bar</p>  <p>• Fixed hybrid bar • Low lingual finish line • Titanium tissue surface • Acrylic resin is processed to the bar</p>		<p>Dolder® Egg Shape Bar</p>  <p>• Removable overdenture design • Anterior clips allow for anterior/posterior rotation of the overdenture • Provides lateral stability to the overdenture</p>	

Introduction



Bars & Frameworks Design Options (Cont'd)

Dolder® U Shape Bar



- Removable overdenture design
- Anterior clips allow for anterior/posterior rotation of the overdenture
- Provides lateral stability to the overdenture

Hader Bar



- Removable overdenture design with clips that engage undercuts
- Provides lateral stability to the overdenture
- 4mm between implants is needed for clips

Primary Bar




- Most secure removable overdenture design
- May be used with attachments or secondary casting
- Bar can be designed with a 2° – 6° taper

Combination Primary Bar With Hader Or Dolder Designs





- Combines a milled bar with Hader or Dolder Designs
- Provides excellent lateral stability to the overdenture
- Bar can be designed with a 2° – 6° taper

Design Features

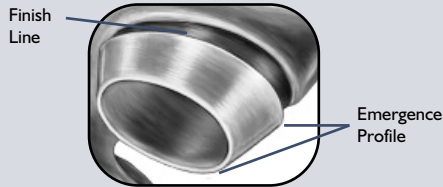

Implant Cylinder Extensions



Stability Struts

Ask for these design features on the BellaTek Bars & Frameworks Work Order Form (ART880).



Copymilled Bar/Framework



- Ideal for both fixed and removable prosthetic designs
- Technician-fabricated resin pattern for porcelain or acrylic resin bonded to titanium

Introduction

Restorative Products Flowchart

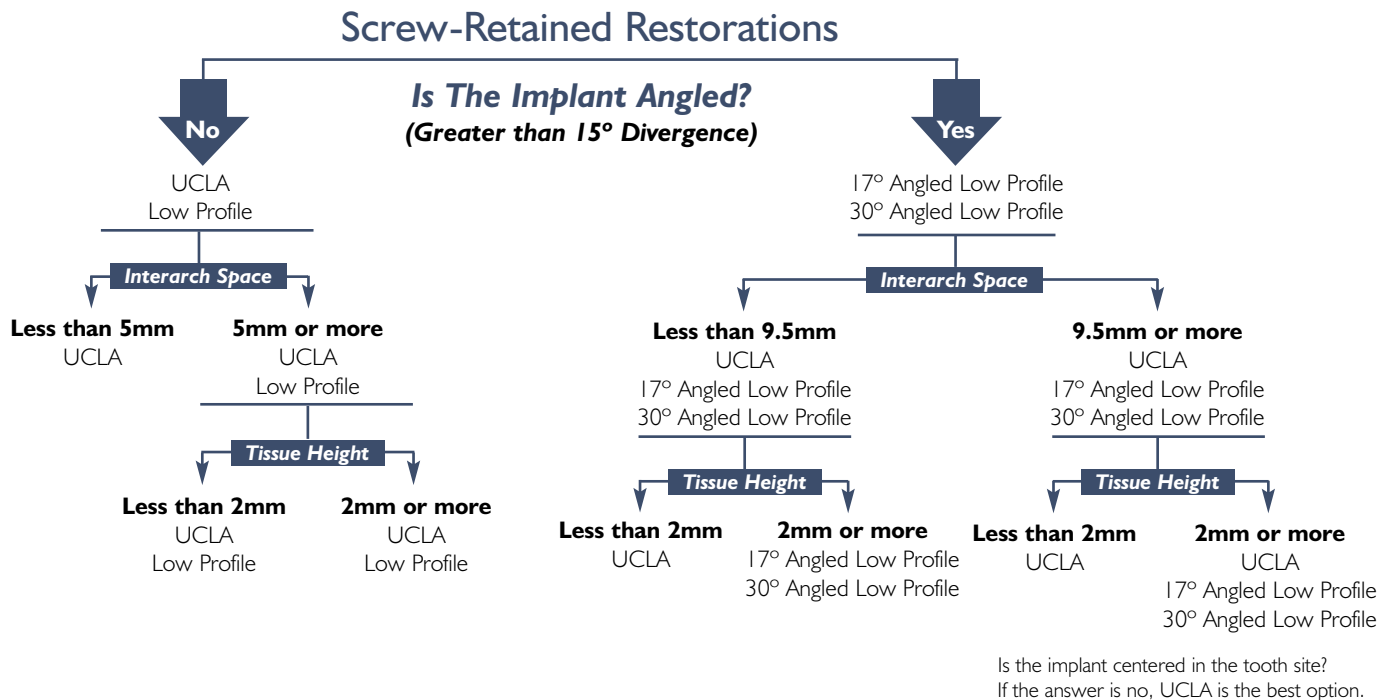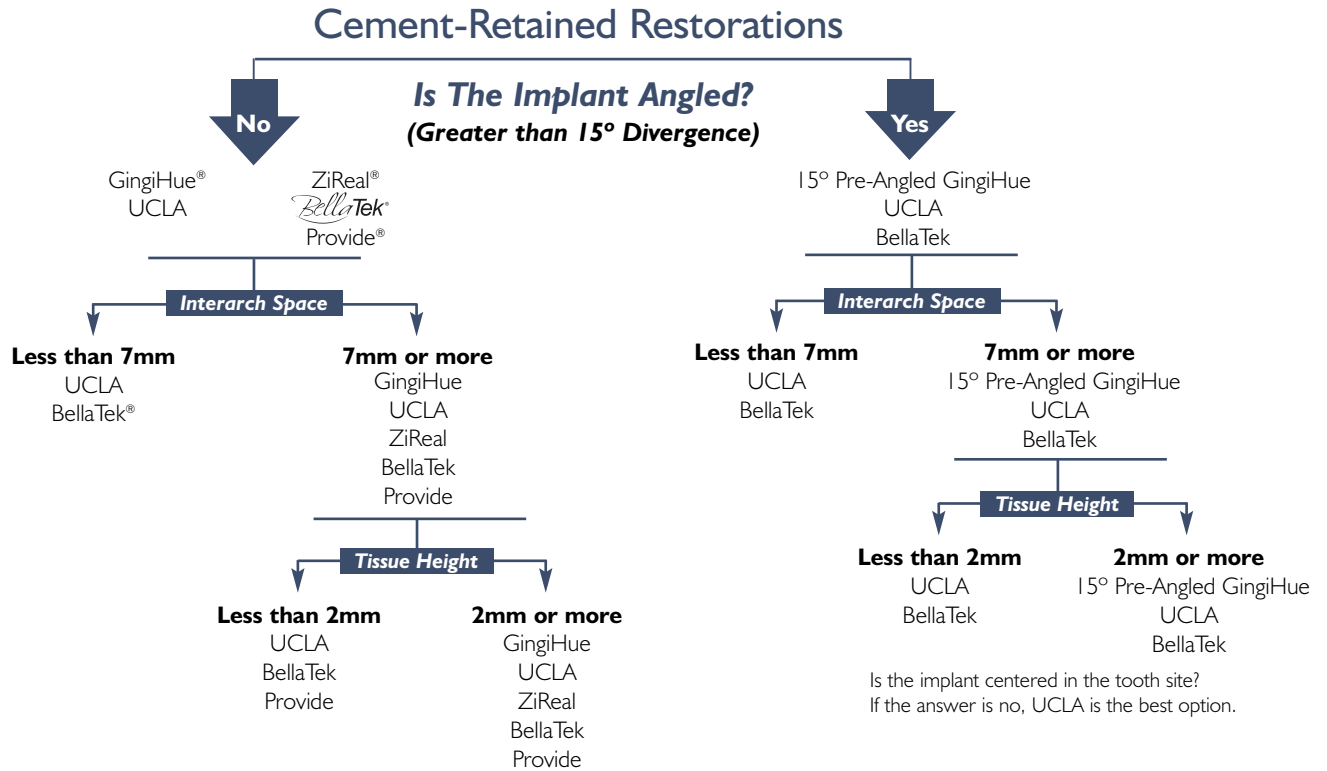

Provisional Restorations

Certain® Internal Connection

PreFormance® Posts

Indications:

- Single and multi-unit provisional cement-retained restorations
- Minimum interarch space of 7mm
- Maximum angulation of 15°
- Intraoral use limited to 180 days
- Immediate nonocclusal loading of single-unit provisional restorations
- Multiple unit restorations will require an evaluation of occlusal forces in lateral and protrusive excursions and masticatory forces to minimize the load on the provisional restorations
- Guided soft-tissue healing of single and multi-unit restorations of integrated implants

Material:

PEEK: Titanium Alloy Connection



3.4mm Seating Surface			
Emergence Profile	Collar Height	Item Numbers (Straight)	Item Numbers (15° Pre-Angled)
3.8mm	4mm	IMPFP34	IMPAPF34
3.8mm	6mm	IMPFP36	IMPAPF36
5mm	4mm	IMPFP354	IMPAPF354
5mm	6mm	IMPFP356	IMPAPF356
4.1mm Seating Surface			
Emergence Profile	Collar Height	Item Numbers (Straight)	Item Numbers (15° Pre-Angled)
5mm	4mm	IPFP454	IPAPF454
5mm	6mm	IPFP456	IPAPF456
5mm Seating Surface			
Emergence Profile	Collar Height	Item Numbers (Straight)	Item Numbers (15° Pre-Angled)
5mm	4mm	IWPFP554	IPAPF554
5mm	6mm	IWPFP556	IPAPF556
6mm Seating Surface			
Emergence Profile	Collar Height	Item Numbers (Straight)	Item Numbers (15° Pre-Angled)
6mm	4mm	IWPFP664	IPAPF664
6mm	6mm	IWPFP666	IPAPF666

All indicated measurements are in millimeters.

Some products may not be available outside of the United States.
 Algunos productos no se comercializan fuera de EE.UU.
 Certains produits ne sont pas disponibles en dehors des États-Unis.
 Einige Produkte sind außerhalb der USA nicht erhältlich.

Provisional Restorations

Certain® Internal Connection

PreFormance® Temporary Cylinders


Indications:

- Single and multi-unit provisional screw-retained restorations
- Minimum interarch space of 6mm
- Maximum angulation of 15°
- Intraoral use limited to 180 days
- Immediate nonocclusal loading of single-unit provisional restorations
- Multiple unit restorations will require an evaluation of prosthesis support to minimize the load on the provisional abutments
- Occlusal loading of single and multi-unit restorations of integrated implants for guided tissue healing

Material:

PEEK: Titanium Alloy Connection

Description	Item Numbers
3.4mm Seating Surface	
Hexed	IMPFTC34
Non-Hexed	IMPFTC32
4.1mm Seating Surface	
Hexed	IPFTC41
Non-Hexed	IPFTC42
5mm Seating Surface	
Hexed	IWPFTC51
Non-Hexed	IWPFTC52
6mm Seating Surface	
Hexed	IWPFTC61
Non-Hexed	IWPFTC62



Titanium Temporary Cylinders


Indications:

- Single and multi-unit provisional screw-retained restorations
- Minimum interarch space of 6mm
- Maximum angulation of 15°
- Immediate nonocclusal loading of single-unit provisional restorations
- Multiple unit restorations will require an evaluation of prosthesis support to minimize the load on the provisional abutments
- Occlusal loading of single and multi-unit restorations of integrated implants for guided tissue healing

Material:

Titanium Alloy Connection

Description	Item Numbers
3.4mm Seating Surface	
Hexed	IMMTCS1
Non-Hexed	—
4.1mm Seating Surface	
Hexed	IITCS41
Non-Hexed	IITCS42
5mm Seating Surface	
Hexed	IWTCS51
Non-Hexed	IWTCS52
6mm Seating Surface	
Hexed	IWTCS61
Non-Hexed	IWTCS62



Some products may not be available outside of the United States.
 Algunos productos no se comercializan fuera de EE.UU.
 Certains produits ne sont pas disponibles en dehors des États-Unis.
 Einige Produkte sind außerhalb der USA nicht erhältlich.

Cement-Retained Restorations

Certain® Internal Connection

GingiHue® Posts

Material: Titanium Alloy

Indications:

- Single and multi-unit porcelain fused-to-metal restorations
- Areas of thin tissue where gingival discoloration is possible
- Preparable to follow gingival contours
- Conventional crown and bridge procedures
- Maximum angulation correction of 15°
- Minimum interarch space of 7mm



3.4mm Seating Surface

Emergence Profile	Collar Height	Item Numbers (Straight)	Item Numbers (15° Pre-Angled)
3.8mm	2mm	IMAP32G	IMPAP32G
3.8mm	4mm	IMAP34G	IMPAP34G
5mm	2mm	IMAP352G	IMPAP352G
5mm	4mm	IMAP354G	IMPAP354G

4.1mm Seating Surface

Emergence Profile	Collar Height	Item Numbers (Straight)	Item Numbers (15° Pre-Angled)
5mm	2mm	IAPP452G	IPAP452G
5mm	4mm	IAPP454G	IPAP454G
6mm	2mm	IAPP462G	IPAP462G
6mm	4mm	IAPP464G	IPAP464G

5mm Seating Surface

Emergence Profile	Collar Height	Item Numbers (Straight)	Item Numbers (15° Pre-Angled)
5mm	2mm	IWPP552G	IPAP552G
5mm	4mm	IWPP554G	IPAP554G
6mm	2mm	IWPP562G	IPAP562G
6mm	4mm	IWPP564G	IPAP564G

6mm Seating Surface

Emergence Profile	Collar Height	Item Numbers (Straight)	Item Numbers (15° Pre-Angled)
6mm	2mm	IWPP662G	IPAP662G
6mm	4mm	IWPP664G	IPAP664G

ZiReal® Posts

Indications:

- Single and multi-unit all ceramic restorations
- Preparable to follow gingival contours
- Minimum interarch space of 7mm
- Aesthetic restorations when tissue is limited
- Maximum angulation of 10°



Material: Zirconia Ceramic With A Titanium Alloy Interface

4.1mm Seating Surface

Emergence Profile	Collar Height	Item Numbers
5mm	4mm	ICAP454*
6mm	4mm	ICAP464*

5mm Seating Surface

Emergence Profile	Collar Height	Item Numbers
6mm	4mm	IWCAP564*

*Includes Certain ZiReal Gold-Tite® Screw (IZSHG) and ZiReal Try-In Screw (IZIRTS).


Some products may not be available outside of the United States.
 Algunos productos no se comercializan fuera de EE.UU.
 Certains produits ne sont pas disponibles en dehors des États-Unis.
 Einige Produkte sind außerhalb der USA nicht erhältlich.

All indicated measurements are in millimeters.

Cement-Retained Restorations

Certain® Internal Connection

GingiHue® & ZiReal® Post Components

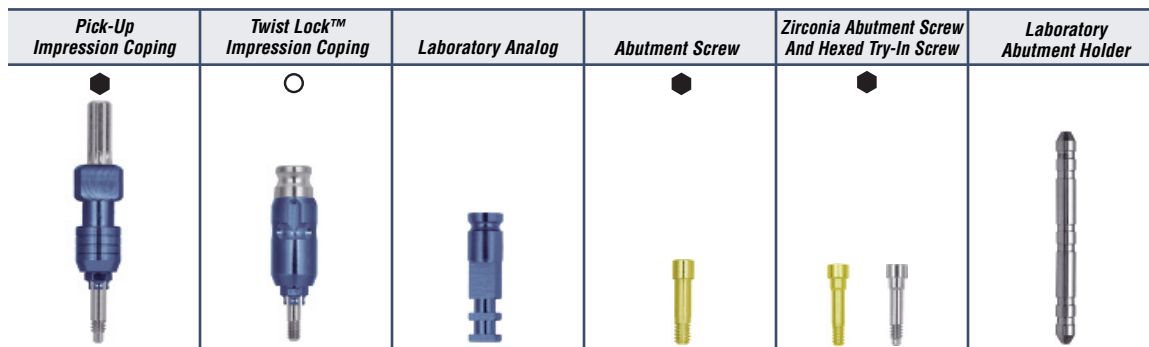

= Requires the use of Hex Driver **PHD02N**, **PHD03N** or Driver Tip **RASH3N**, **RASH8N**
 = Requires the use of Impression Coping Driver **ICD00**

Description	3.4mm			4.1mm			5mm			6mm	
	3.4	3.8	5.0	4.1	5.0	6.0	5.0	5.6	6.0	6.0	6.8
Pick-Up Impression Coping	IMIC30	IMIC33	IMIC35	IIC41 IIC42*	IIC12	IIC60	IWIP50	IWIP55	IWIP56	IWIP60	IWIP66
Twist Lock Impression Coping		IMIT33	IMIT35	IIC44	IIC45	IIC46	IWIT50	IWIT55	IWIT56	IWIT60	IWIT66
Laboratory Analog		IMMILA			IILA20			IILAW5			IILAW6
Abutment Screw	IUNIHG**, IUNIHT										
Zirconia Abutment Screw	IZSHG (included with ZiReal Post)										
Zirconia Try-In Screw	IZIRTS (included with ZiReal Post)										
Hexed Try-In Screw (5-pack)	IUNITS										
Laboratory Abutment Holder	ILTAH57										

*Non-Hexed
 **Recommended

Certain Internal Connection

Some products may not be available outside of the United States.
 Algunos productos no se comercializan fuera de EE.UU.
 Certains produits ne sont pas disponibles en dehors des États-Unis.
 Einige Produkte sind außerhalb der USA nicht erhältlich.

Cement-Retained Restorations

Certain® Internal Connection

UCLA Abutments

Indications:


- Laboratory fabricated custom abutments
- Single and multi-unit restorations
- Minimum interarch space of 6mm
- For aesthetic restorations when tissue is limited
- Maximum angulation correction of 30°

Material:

Machined Gold Alloy Cylinder With Plastic Unitube



Description	Item Numbers
3.4mm Seating Surface Gold (Hexed)	IMUCG1C
4.1mm Seating Surface Gold (Hexed)	IGUCA1C
5mm Seating Surface Gold (Hexed)	IWGA51C
6mm Seating Surface Gold (Hexed)	IWGA61C




All indicated measurements are in millimeters.

Some products may not be available outside of the United States.
 Algunos productos no se comercializan fuera de EE.UU.
 Certains produits ne sont pas disponibles en dehors des États-Unis.
 Einige Produkte sind außerhalb der USA nicht erhältlich.

Cement-Retained Restorations

Certain® Internal Connection

UCLA Abutment Components

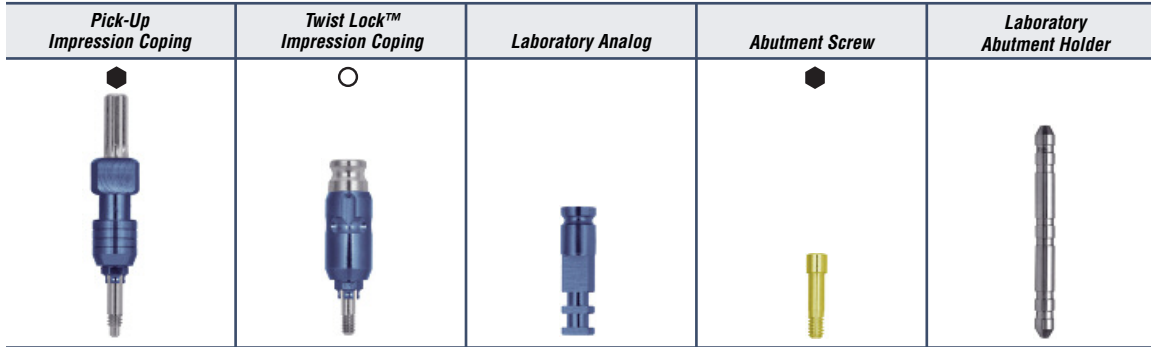

= Requires the use of Hex Driver **PHD02N**, **PHD03N** or Driver Tip **RASH3N**, **RASH8N**
 = Requires the use of Impression Coping Driver **ICD00**

Description	3.4mm			4.1mm			5mm			6mm	
	3.4	3.8	5.0	4.1	5.0	6.0	5.0	5.6	6.0	6.0	6.8
Pick-Up Impression Coping	IMIC30	IMIC33	IMIC35	IIIC41 IIIC42*	IIIC12	IIIC60	IWIP50	IWIP55	IWIP56	IWIP60	IWIP66
Twist Lock Impression Coping		IMIT33	IMIT35	IIIC44	IIIC45	IIIC46	IWIT50	IWIT55	IWIT56	IWIT60	IWIT66
Laboratory Analog		IMMILA			IILA20			IILAW5		IILAW6	
Abutment Screw	IUNIHG**, IUNIHT										
Hexed Try-In Screw (5-pack)	IUNITS										
Laboratory Abutment Holder	ILTAH57										

*Non-Hexed
 **Recommended

Gold Alloy Cylinder Formulation	
Melting Range	1400–1490°C (2550–2710°F)
Solidus	1400°C
Liquidus	1490°C
CTE	13.5 x 10 ⁻⁶ K at 500°C

An alloy with a CTE of 10⁻⁶K at 500°C is recommended.

Some products may not be available outside of the United States.
 Algunos productos no se comercializan fuera de EE.UU.
 Certains produits ne sont pas disponibles en dehors des États-Unis.
 Einige Produkte sind außerhalb der USA nicht erhältlich.

Cement-Retained Restorations

Certain® Internal Connection

Provide® Abutments

Indications:


- Single and multi-unit porcelain fused-to-metal restorations
- Fixed margin abutments
- Snap-on impression components
- Maximum angulation correction of 10°
- Minimum interarch space of 7mm

Material:
Titanium Alloy


4.1mm Seating Surface			Item Numbers		
Emergence Profile	Collar Height	Post Height	Abutment Placement Kit	Abutment Restorative Kit	Abutment Only
4.8mm	1mm	4mm	PAK4140*	PRK484**	IPA4140
4.8mm	2mm	4mm	PAK4240*	PRK484**	IPA4240
4.8mm	3mm	4mm	PAK4340*	PRK484**	IPA4340
4.8mm	4mm	4mm	PAK4440*	PRK484**	IPA4440
4.8mm	1mm	5.5mm	PAK4155*	PRK485**	IPA4155
4.8mm	2mm	5.5mm	PAK4255*	PRK485**	IPA4255
4.8mm	3mm	5.5mm	PAK4355*	PRK485**	IPA4355
4.8mm	4mm	5.5mm	PAK4455*	PRK485**	IPA4455



5mm Seating Surface			Item Numbers		
Emergence Profile	Collar Height	Post Height	Abutment Placement Kit	Abutment Restorative Kit	Abutment Only
6.5mm	1mm	4mm	PAK5140*	PRK654**	IPA5140
6.5mm	2mm	4mm	PAK5240*	PRK654**	IPA5240
6.5mm	3mm	4mm	PAK5340*	PRK654**	IPA5340
6.5mm	4mm	4mm	PAK5440*	PRK654**	IPA5440
6.5mm	1mm	5.5mm	PAK5155*	PRK655**	IPA5155
6.5mm	2mm	5.5mm	PAK5255*	PRK655**	IPA5255
6.5mm	3mm	5.5mm	PAK5355*	PRK655**	IPA5355
6.5mm	4mm	5.5mm	PAK5455*	PRK655**	IPA5455



6mm Seating Surface			Item Numbers		
Emergence Profile	Collar Height	Post Height	Abutment Placement Kit	Abutment Restorative Kit	Abutment Only
6.5mm	1mm	4mm	PAK6140*	PRK654**	IPA6140
6.5mm	2mm	4mm	PAK6240*	PRK654**	IPA6240
6.5mm	3mm	4mm	PAK6340*	PRK654**	IPA6340
6.5mm	4mm	4mm	PAK6440*	PRK654**	IPA6440
6.5mm	1mm	5.5mm	PAK6155*	PRK655**	IPA6155
6.5mm	2mm	5.5mm	PAK6255*	PRK655**	IPA6255
6.5mm	3mm	5.5mm	PAK6355*	PRK655**	IPA6355
6.5mm	4mm	5.5mm	PAK6455*	PRK655**	IPA6455



*Abutment Placement Kit includes the Provide Abutment, Protection Cap and Certain® Gold-Tite® Hexed Screw IUNIHG.

**Abutment Restorative Kit includes Impression Coping, Impression Coping w/Holes, Waxing Sleeve (single-unit), Waxing Sleeve (multi-unit) and Non-Prepared Analog.

Some products may not be available outside of the United States.
 Algunos productos no se comercializan fuera de EE.UU.
 Certains produits ne sont pas disponibles en dehors des États-Unis.
 Einige Produkte sind außerhalb der USA nicht erhältlich.

Cement-Retained Restorations


Certain® Internal Connection

Provide® Abutment Components



Description	4mm Post Height		5.5mm Post Height		
	4.8	6.5	4.8	6.5	
Protection Cap	PPC484	PPC654	PPC485	PPC655	
Impression Coping (Unprepared)	▶ PIC484	▶ PIC654	▶ PIC485	▶ PIC655	
Impression Coping W/Holes (Prepared)	PIC484H	PIC654H	PIC485H	PIC655H	
Abutment Analog (Unprepared)	▶ PAA484	▶ PAA654	▶ PAA485	▶ PAA655	
Abutment Analog W/Pin (Prepared)	PAAP48	PAAP65	PAAP48	PAAP65	
Abutment Screw	IUNIHG*, IUNIHT				
Waxing Sleeve	single-unit >	PWS48S	PWS65S	PWS48S	PWS65S
	multi-unit >	PWS48M	PWS65M	PWS48M	PWS65M
Temporary Cylinder	single-unit >	PUA48S	PUA65S	PUA48S	PUA65S
	multi-unit >	PUA48M	PUA65M	PUA48M	PUA65M

*Recommended

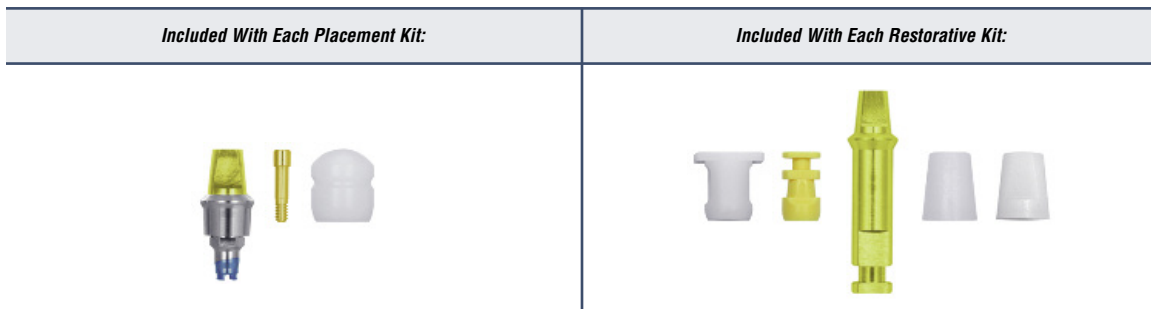

Some products may not be available outside of the United States.
 Algunos productos no se comercializan fuera de EE.UU.
 Certains produits ne sont pas disponibles en dehors des États-Unis.
 Einige Produkte sind außerhalb der USA nicht erhältlich.

Screw-Retained Restorations

Certain® Internal Connection

UCLA Abutments

Indications:


- Single and multi-unit restorations
- Minimum interarch space of 4mm
- For aesthetic restorations when tissue is limited

Material:

Machined Gold Alloy Cylinder With Plastic Unitube



Description	Item Numbers
3.4mm Seating Surface	
Gold (Hexed)	IMUCG1C*
Gold (Non-Hexed)	IMUCG2C
Gold (Non-Hexed)	IMUCG2T
Castable (Non-Hexed)	IMUCC2C
Castable (Non-Hexed)	IMUCC2T
4.1mm Seating Surface	
Gold (Hexed)	IGUCA1C*
Gold (Non-Hexed)	IGUCA2C
Gold (Non-Hexed)	IGUCA2T
Gold Standard ZR (Hexed)	—
Castable (Hexed)	—
Castable (Non-Hexed)	IUNAB2C
Castable (Non-Hexed)	IUNAB2T
Castable (Hexed) 25-pack	—
Castable (Non-Hexed) 25-pack	—
5mm Seating Surface	
Gold (Hexed)	IWGA51C*
Gold (Non-Hexed)	IWGA52C
Gold (Non-Hexed)	IWGA52T
Gold Standard ZR (Hexed)	—
Castable (Hexed)	—
Castable (Non-Hexed)	IWPC52C
Castable (Non-Hexed)	IWPC52T
6mm Seating Surface	
Gold (Hexed)	IWGA61C*
Gold (Non-Hexed)	IWGA62C
Gold (Non-Hexed)	IWGA62T
Gold Standard ZR (Hexed)	—
Castable (Hexed)	—
Castable (Non-Hexed)	IWPC62C
Castable (Non-Hexed)	IWPC62T

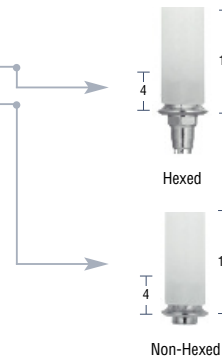

*UCLA Gold Hexed Abutments do not include the screw. The final Gold-Tite® Screw (IUNIHG) or the Titanium Screw (IUNIHT) must be ordered separately.


All indicated measurements are in millimeters.

Some products may not be available outside of the United States.
 Algunos productos no se comercializan fuera de EE.UU.
 Certains produits ne sont pas disponibles en dehors des États-Unis.
 Einige Produkte sind außerhalb der USA nicht erhältlich.

Screw-Retained Restorations

Certain® Internal Connection

UCLA Abutment Components

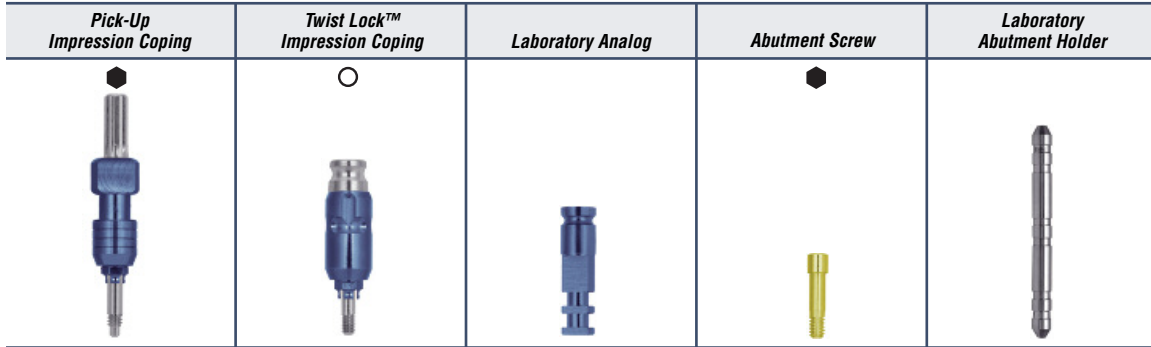

= Requires the use of Hex Driver **PHD02N**, **PHD03N** or Driver Tip **RASH3N**, **RASH8N**
 = Requires the use of Impression Coping Driver **ICD00**

Description	3.4mm			4.1mm			5mm			6mm	
	3.4	3.8	5.0	4.1	5.0	6.0	5.0	5.6	6.0	6.0	6.8
Pick-Up Impression Coping	IMIC30	IMIC33	IMIC35	IIIC41 IIIC42*	IIIC12	IIIC60	IWIP50	IWIP55	IWIP56	IWIP60	IWIP66
Twist Lock Impression Coping		IMIT33	IMIT35	IIIC44	IIIC45	IIIC46	IWIT50	IWIT55	IWIT56	IWIT60	IWIT66
Laboratory Analog		IMMILA		IILA20			IILAW5			IILAW6	
Abutment Screw	Hexed: IUNIHT, IUNIHG**, Non-Hexed: ILRGHG**, ILRGHT										
Hexed Try-In Screw (5-pack)	IUNITS (for hexed only)										
Laboratory Abutment Holder	ILTAH57										

*Non-Hexed
 **Recommended

Gold Alloy Cylinder Formulation	
Melting Range	1400–1490°C (2550–2710°F)
Solidus	1400°C
Liquidus	1490°C
CTE	13.5 x 10 ⁻⁶ °K at 500°C

An alloy with a CTE of 10⁻⁶°K at 500°C is recommended.

Some products may not be available outside of the United States.
 Algunos productos no se comercializan fuera de EE.UU.
 Certains produits ne sont pas disponibles en dehors des États-Unis.
 Einige Produkte sind außerhalb der USA nicht erhältlich.

Screw-Retained Restorations

Certain® Internal Connection


Low Profile Abutments

Indications:

- Single and multi-unit screw-retained restorations
- Minimum interarch space of 7.5mm
- Minimum tissue height of 1mm
- Angle correction up to 30°

Material:

Titanium Alloy

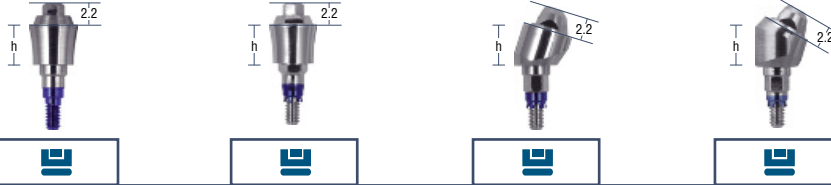

3.4mm Seating Surface		Item Numbers			
Collar Height	Straight (Non-Hexed)	Straight (Hexed)	17° Pre-Angled (Hexed)	30° Pre-Angled (Hexed)	
1mm	ILPC341U	ILPC341	—	—	
2mm	ILPC342U	ILPC342	ILPAC3217	—	
3mm	ILPC343U	ILPC343	—	ILPAC3330	
4mm	ILPC344U	ILPC344	ILPAC3417	—	
5mm	—	—	—	ILPAC3530	

4.1mm Seating Surface		Item Numbers			
Collar Height	Straight (Non-Hexed)	Straight (Hexed)	17° Pre-Angled (Hexed)	30° Pre-Angled (Hexed)	
1mm	ILPC441U	ILPC441	—	—	
2mm	ILPC442U	ILPC442	ILPAC4217	—	
3mm	ILPC443U	ILPC443	—	ILPAC4330	
4mm	ILPC444U	ILPC444	ILPAC4417	—	
5mm	—	—	—	ILPAC4530	

5mm Seating Surface		Item Numbers			
Collar Height	Straight (Non-Hexed)	Straight (Hexed)	17° Pre-Angled (Hexed)	30° Pre-Angled (Hexed)	
1mm	ILPC541U	ILPC541	—	—	
2mm	ILPC542U	ILPC542	ILPAC5217	—	
3mm	ILPC543U	ILPC543	—	ILPAC5330	
4mm	ILPC544U	ILPC544	ILPAC5417	—	
5mm	—	—	—	ILPAC5530	











All indicated measurements are in millimeters.

Some products may not be available outside of the United States.
 Algunos productos no se comercializan fuera de EE.UU.
 Certains produits ne sont pas disponibles en dehors des États-Unis.
 Einige Produkte sind außerhalb der USA nicht erhältlich.

Screw-Retained Restorations

Certain® Internal Connection

Low Profile Abutment Components

<i>Pick-Up Impression Coping</i>	<i>Twist Lock™ Impression Coping</i>	<i>Laboratory Analog</i>	<i>Healing Cap</i>	<i>Gold And Castable Cylinder</i>
				
<i>QuickBridge®</i>	<i>Temporary Cylinder</i>	<i>Polishing Protector</i>	<i>Retaining Screw</i>	<i>Driver And Driver Tip</i>
				

◆ = Requires the use of Hex Driver **PHD02N**, **PHD03N** or Driver Tip **RASH3N**, **RASH8N**

○ = Requires the use of Impression Coping Driver **ICD00**

Description		4.8mm Restorative Platform
Pick-Up Impression Coping	hexed > non-hexed >	LPCPIC1 LPCPIC2
Twist Lock Impression Coping	hexed > non-hexed >	LPCTIC1 LPCTIC2
QuickBridge Impression Coping		LPCRIC
Laboratory Analog		LPCLA
Temporary Cylinder	hexed > non-hexed >	LPCTC1 LPCTC2
Healing Cap		LPCHC
PreFormance® Temp. Cylinder	hexed > non-hexed >	LPCPTC1 LPCPTC2
QuickBridge		LPCQB
QuickBridge Replacement Cap		LPCQBCAP
Distal Extension		LPCDE
Gold Cylinder	hexed > non-hexed >	LPCGC1 LPCGC2
Castable Cylinder	hexed > non-hexed >	LPCCC1 LPCCC2
Laser Welded Cylinder		LPCTUCA
Waxing Screw		LPCWS
Retaining Screw		LPCGSH, LPCTSH
Lapping Tool		LPCAMI
Polishing Protector		LPCPP

Abutment Compatibility

Component	Hexed Abutment	Non-Hexed Abutment
Hexed	Yes	No
Non-Hexed	Yes	Yes

Some products may not be available outside of the United States.
 Algunos productos no se comercializan fuera de EE.UU.
 Certains produits ne sont pas disponibles en dehors des États-Unis.
 Einige Produkte sind außerhalb der USA nicht erhältlich.

Overdenture Restorations

Certain® Internal Connection

LOCATOR® Abutments

Indications:

- Tissue supported removable overdentures on 2-4 implants
- Partially edentulous overdentures with one or more implants
- Limited interarch distance
- Angle correction with up to 40° between divergent implants

Material:


Abutment: Titanium Alloy With Titanium Nitride Coating
 Housing: Titanium Alloy
 Males: Nylon

3.4mm Seating Surface		Item Numbers
Collar Height		
1mm		IMLOA001
2mm		IMLOA002
3mm		IMLOA003
4mm		IMLOA004
5mm		IMLOA005
6mm		IMLOA006

4.1mm Seating Surface		Item Numbers
Collar Height		
1mm		ILOA001
2mm		ILOA002
3mm		ILOA003
4mm		ILOA004
5mm		ILOA005
6mm		ILOA006



Included With Each Abutment:

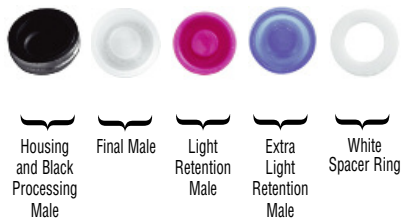





All indicated measurements are in millimeters.

Some products may not be available outside of the United States.
 Algunos productos no se comercializan fuera de EE.UU.
 Certains produits ne sont pas disponibles en dehors des États-Unis.
 Einige Produkte sind außerhalb der USA nicht erhältlich.

Overdenture Restorations

Certain® Internal Connection

LOCATOR® Abutment Components

Impression Coping	Laboratory Analog	Retention Males	Core Tool / Driver And Driver Tip
			

Description	Item Numbers
Impression Coping	LAIC1
Laboratory Analog	LALA1
Extra Light Retention Males (4-pack) - Blue, 1.5lbs/680g	LAELM
Extended Range Males (4-pack) - Green, 4lbs/1800g	LAERM
Extra Light Retention Extended Range Males - Red, 1.5lbs/680g	LELARM
Replacement Males (4-pack) - White, 5lbs/2250g	LARMS
Light Retention Replacement Males (4-pack) - Pink, 3lbs/1350g	LLRMS
Replacement Housing	LOAH
Replacement Housing Kit	LORHK*
Core Tool/Abutment Driver	LCTDR1
Driver Tip 24mm(L)	LOADT4
Driver Tip 30mm(L)	LOADT9
1.25mm/.050in. Driver Tip 24mm(L) - used with LCTDR1	RASH4
1.25mm/.050in. Driver Tip 30mm(L) - used with LCTDR1	RASH9
LOCATOR Bar Attachment	LOAB
LOCATOR Bar Attachment Tap	LOAT
LOCATOR Bar Attachment Drill	LOAD

*Included With **LORHK**
Replacement Housing Kit:



Some products may not be available outside of the United States.
Algunos productos no se comercializan fuera de EE.UU.
Certains produits ne sont pas disponibles en dehors des États-Unis.
Einige Produkte sind außerhalb der USA nicht erhältlich.

Provisional Restorations

External Hex Connection

PreFormance® Posts

Indications:

- Single and multi-unit provisional cement-retained restorations
- Minimum interarch space of 7mm
- Maximum angulation of 15°
- Intraoral use limited to 180 days
- Immediate nonocclusal loading of single-unit provisional restorations
- Multi-unit restorations will require an evaluation of occlusal forces in lateral and protrusive excursions and masticatory forces to minimize the load on the provisional restorations
- Guided soft-tissue healing of single and multi-unit restorations of integrated implants

Material:

PEEK: Titanium Alloy Connection



3.4mm Seating Surface			
Emergence Profile	Collar Height	Item Numbers (Straight)	Item Numbers (15° Pre-Angled)
3.8mm	4mm	MPFP34	MPAPF34
3.8mm	6mm	MPFP36	MPAPF36
4.1mm Seating Surface			
Emergence Profile	Collar Height	Item Numbers (Straight)	Item Numbers (15° Pre-Angled)
5mm	4mm	PFP454	PAPF454
5mm	6mm	PFP456	PAPF456
5mm Seating Surface			
Emergence Profile	Collar Height	Item Numbers (Straight)	Item Numbers (15° Pre-Angled)
5mm	4mm	WPFP554	PAPF554
5mm	6mm	WPFP556	PAPF556
6mm Seating Surface			
Emergence Profile	Collar Height	Item Numbers (Straight)	Item Numbers (15° Pre-Angled)
6mm	4mm	WPFP664	PAPF664
6mm	6mm	WPFP666	PAPF666

All PreFormance Posts are packaged with a Titanium Hexed Screw (UNIHT).

All indicated measurements are in millimeters.

Some products may not be available outside of the United States.
 Algunos productos no se comercializan fuera de EE.UU.
 Certains produits ne sont pas disponibles en dehors des États-Unis.
 Einige Produkte sind außerhalb der USA nicht erhältlich.

Provisional Restorations

External Hex Connection

PreFormance® Temporary Cylinders

Indications:


- Single and multi-unit provisional screw-retained restorations
- Minimum interarch space of 6mm
- Maximum angulation of 15°
- Intraoral use limited to 180 days
- Immediate nonocclusal loading of single-unit provisional restorations
- Multi-unit restorations will require an evaluation of prosthesis support to minimize the load on the provisional abutments
- Occlusal loading of single and multi-unit restorations of integrated implants for guided tissue healing

Material:

PEEK: Titanium Alloy Connection



Description	Item Numbers
3.4mm Seating Surface	
Hexed	MPFTC34
Non-Hexed	MPFTC32
4.1mm Seating Surface	
Hexed	PFTC41
Non-Hexed	PFTC42
5mm Seating Surface	
Hexed	WPFTC51
Non-Hexed	WPFTC52
6mm Seating Surface	
Hexed	WPFTC61
Non-Hexed	WPFTC62



All PreFormance Cylinders are packaged with a Titanium Hexed Screw (UNIHT).

Titanium Temporary Cylinders

Indications:


- Single and multi-unit provisional screw-retained restorations
- Minimum interarch space of 6mm
- Maximum angulation of 15°
- Immediate nonocclusal loading of single-unit provisional restorations
- Multi-unit restorations will require an evaluation of prosthesis support to minimize the load on the provisional abutments
- Occlusal loading of single and multi-unit restorations of integrated implants for guided tissue healing

Material:

Titanium Alloy Connection



Description	Item Numbers
3.4mm Seating Surface	
Hexed	MMTCS1
Non-Hexed	—
4.1mm Seating Surface	
Hexed	ITCS41
Non-Hexed	ITCS42
5mm Seating Surface	
Hexed	WTCS51
Non-Hexed	WTCS52
6mm Seating Surface	
Hexed	WTCS61
Non-Hexed	WTCS62



All indicated measurements are in millimeters.

Some products may not be available outside of the United States.

Cement-Retained Restorations

External Hex Connection


GingiHue® Posts

Indications:

- Single and multi-unit porcelain fused-to-metal restorations
- Areas of thin tissue where gingival discoloration is possible
- Preparable to follow gingival contours
- Conventional crown and bridge procedures
- Maximum angulation correction of 15°
- Minimum interarch space of 7mm

Material:

Straight Post (Commercially Pure Titanium)
Pre-Angled Post (Titanium Alloy)



3.4mm Seating Surface		Item Numbers (Straight)	Item Numbers (15° Pre-Angled)
Emergence Profile	Collar Height		
3.8mm	2mm	MAP32G	MPAP32G
3.8mm	4mm	MAP34G	MPAP34G
4.1mm Seating Surface		Item Numbers (Straight)	Item Numbers (15° Pre-Angled)
Emergence Profile	Collar Height		
5mm	2mm	APP452G	PAP452G
5mm	4mm	APP454G	PAP454G
6mm	2mm	APP462G	PAP462G
6mm	4mm	APP464G	PAP464G
5mm Seating Surface		Item Numbers (Straight)	Item Numbers (15° Pre-Angled)
Emergence Profile	Collar Height		
5mm	2mm	WPP552G	PAP552G
5mm	4mm	WPP554G	PAP554G
6mm	2mm	WPP562G	PAP562G
6mm	4mm	WPP564G	PAP564G
6mm Seating Surface		Item Numbers (Straight)	Item Numbers (15° Pre-Angled)
Emergence Profile	Collar Height		
6mm	2mm	WPP662G	PAP662G
6mm	4mm	WPP664G	PAP664G

ZiReal® Posts

Indications:

- Single and multi-unit all ceramic restorations
- Preparable to follow gingival contours
- Minimum interarch space of 7mm
- Aesthetic restorations when tissue is limited
- Maximum angulation of 10°

Material: Zirconia Ceramic With A Titanium Alloy Interface



4.1mm Seating Surface		Item Numbers
Emergence Profile	Collar Height	
5mm	4mm	CAP454
6mm	4mm	CAP464
5mm Seating Surface		Item Numbers
Emergence Profile	Collar Height	
6mm	4mm	WCAP564


All indicated measurements are in millimeters.

Some products may not be available outside of the United States.
Algunos productos no se comercializan fuera de EE.UU.
Certains produits ne sont pas disponibles en dehors des États-Unis.
Einige Produkte sind außerhalb der USA nicht erhältlich.

Cement-Retained Restorations

External Hex Connection

GingiHue® & ZiReal® Post Components

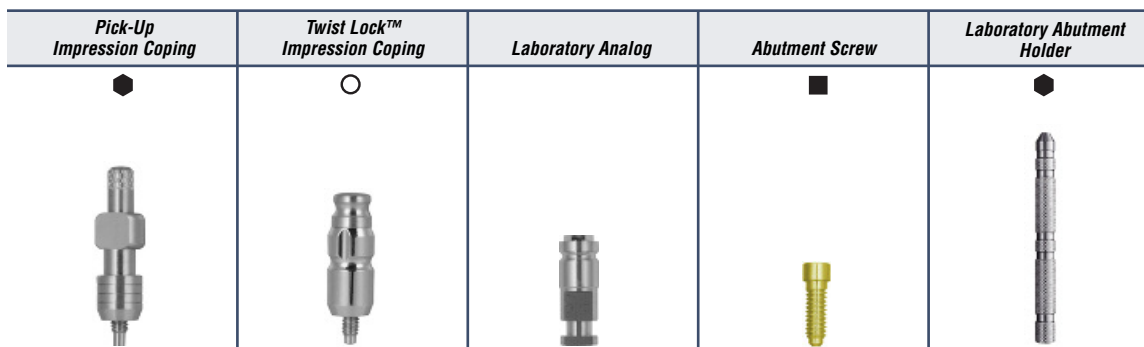

◆ = Requires the use of Hex Driver **PHD02N**, **PHD03N** or Driver Tip **RASH3N**, **RASH8N**

○ = Requires the use of Impression Coping Driver **ICD00**

■ = Requires the use of Square Driver **PSQD0N**, **PSQD1N** or Driver Tip **RASQ3N**, **RASQ8N**

Description	3.4mm	4.1mm		5mm		6mm
Emergence Profile	3.8	5.0	6.0	5.0	6.0	6.0
Pick-Up Impression Coping	MIC33	IIC12	IIC60	WIP55	WIP56	WIP66
Twist Lock Impression Coping	—	IIC45	IIC46	WIT55	WIT56	WIT66
Laboratory Analog	MMILA	ILA20		ILAW5		ILAW6
Abutment Screw	UNISG*, UNIHG, UNIHT					
Square Try-In Screw (5-pack)	MUNITS	UNITS				
Laboratory Abutment Holder	LTAH5	LTAH7				

*Recommended

Some products may not be available outside of the United States.
 Algunos productos no se comercializan fuera de EE.UU.
 Certains produits ne sont pas disponibles en dehors des États-Unis.
 Einige Produkte sind außerhalb der USA nicht erhältlich.

Cement-Retained Restorations

External Hex Connection

UCLA Abutments

Indications:


- Laboratory fabricated custom abutments
- Single and multi-unit restorations
- Minimum interarch space of 6mm
- For aesthetic restorations when tissue is limited
- Maximum angulation correction of 30°

Material:

Machined Gold Alloy Cylinder With Plastic Unitube



Description	Item Numbers
3.4mm Seating Surface	
Gold (Hexed)	MUCG1C
4.1mm Seating Surface	
Gold (Hexed)	GUCA1C
Gold Standard ZR (Hexed)	SGUCA1C
Castable (Hexed)	UNAB1C
Castable (Hexed) 25-pack	UNA125
5mm Seating Surface	
Gold (Hexed)	WGA51C
Gold Standard ZR (Hexed)	SWGA51C
Castable (Hexed)	WPC51C
6mm Seating Surface	
Gold (Hexed)	WGA61C
Gold Standard ZR (Hexed)	SWGA61C
Castable (Hexed)	WPC61C




All indicated measurements are in millimeters.

Some products may not be available outside of the United States.
 Algunos productos no se comercializan fuera de EE.UU.
 Certains produits ne sont pas disponibles en dehors des États-Unis.
 Einige Produkte sind außerhalb der USA nicht erhältlich.

Cement-Retained Restorations

External Hex Connection

UCLA Abutment Components

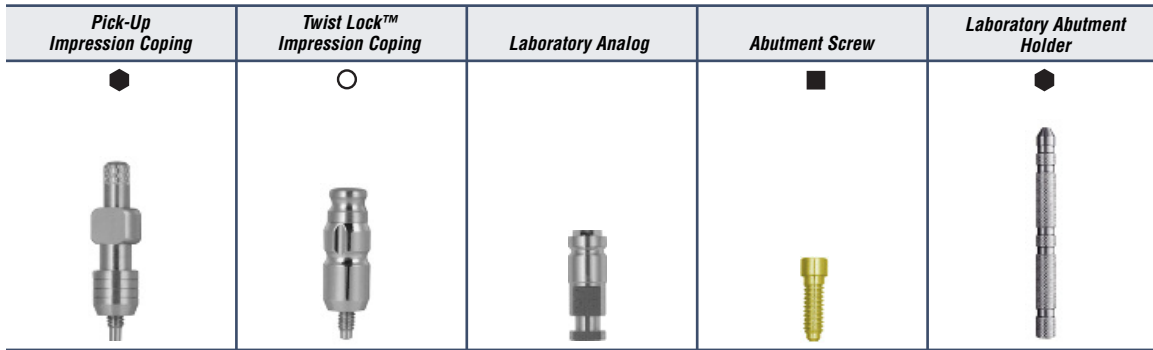

= Requires the use of Hex Driver **PHD02N**, **PHD03N** or Driver Tip **RASH3N**, **RASH8N**
 = Requires the use of Impression Coping Driver **ICD00**
 = Requires the use of Square Driver **PSQD0N**, **PSQD1N** or Driver Tip **RASQ3N**, **RASQ8N**

Description	3.4mm		4.1mm		5mm		6mm
	3.8	5.0	6.0	5.0	6.0	6.0	
Emergence Profile							
Pick-Up Impression Coping	MIC33	IIC12	IIC60	WIP55	WIP56	WIP66	
Twist Lock Impression Coping	—	IIC45	IIC46	WIT55	WIT56	WIT66	
Laboratory Analog	MMILA	ILA20		ILAW5		ILAW6	
Abutment Screw	UNISG*, UNIHG, UNIHT						
Square Try-In Screw (5-pack)	MUNITS						UNITS
Laboratory Abutment Holder	LTAH5						LTAH7

*Recommended

Gold Alloy Cylinder Formulation	
Melting Range	1400–1490°C (2550–2710°F)
Solidus	1400°C
Liquidus	1490°C
CTE	13.5 x 10 ⁻⁶ /K at 500°C

An alloy with a CTE of 10⁻⁶/K at 500°C is recommended.

Some products may not be available outside of the United States.
 Algunos productos no se comercializan fuera de EE.UU.
 Certains produits ne sont pas disponibles en dehors des États-Unis.
 Einige Produkte sind außerhalb der USA nicht erhältlich.

Screw-Retained Restorations

External Hex Connection

UCLA Abutments

Indications:


- Single and multi-unit restorations
- Minimum interarch space of 4mm
- For aesthetic restorations when tissue is limited

Material:

Machined Gold Alloy Cylinder With Plastic Unitube



Description	Item Numbers
3.4mm Seating Surface	
Gold (Hexed)	MUCG1C
Gold (Non-Hexed)	MUCG2C
Gold (Non-Hexed)	—
Castable (Hexed)	MUCC1C
Castable (Non-Hexed)	MUCC2C
Castable (Non-Hexed)	—
4.1mm Seating Surface	
Gold (Hexed)	GUCA1C
Gold (Non-Hexed)	GUCA2C
Gold (Non-Hexed)	—
Gold Standard ZR (Hexed)	SGUCA1C
Castable (Hexed)	UNAB1C
Castable (Non-Hexed)	UNAB2C
Castable (Non-Hexed)	—
Castable (Hexed) 25-pack	UNA125
Castable (Non-Hexed) 25-pack	UNA225
5mm Seating Surface	
Gold (Hexed)	WGA51C
Gold (Non-Hexed)	WGA52C
Gold (Non-Hexed)	—
Gold Standard ZR (Hexed)	SWGA51C
Castable (Hexed)	WPC51C
Castable (Non-Hexed)	WPC52C
Castable (Non-Hexed)	—
6mm Seating Surface	
Gold (Hexed)	WGA61C
Gold (Non-Hexed)	WGA62C
Gold (Non-Hexed)	—
Gold Standard ZR (Hexed)	SWGA61C
Castable (Hexed)	WPC61C
Castable (Non-Hexed)	WPC62C
Castable (Non-Hexed)	—

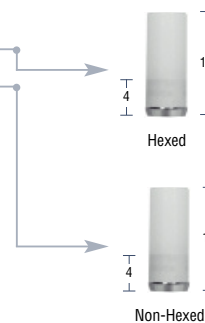


All indicated measurements are in millimeters.

Some products may not be available outside of the United States.
 Algunos productos no se comercializan fuera de EE.UU.
 Certains produits ne sont pas disponibles en dehors des États-Unis.
 Einige Produkte sind außerhalb der USA nicht erhältlich.

Screw-Retained Restorations

External Hex Connection

UCLA Abutment Components

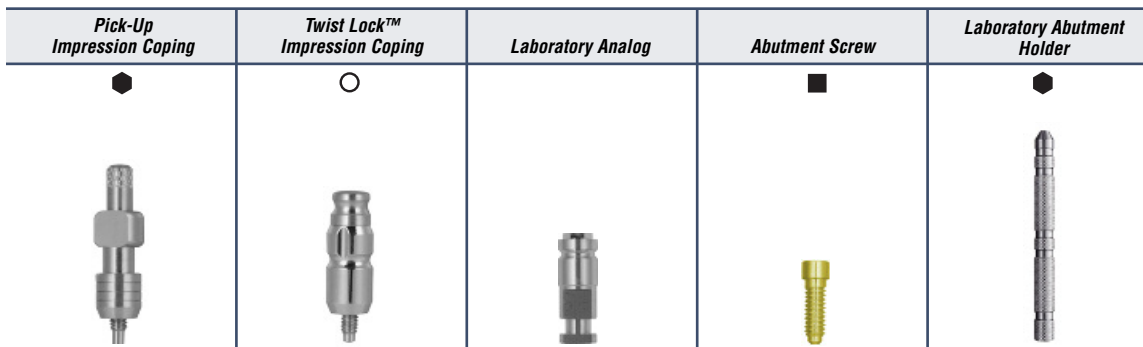

◆ = Requires the use of Hex Driver **PHD02N**, **PHD03N** or Driver Tip **RASH3N**, **RASH8N**

○ = Requires the use of Impression Coping Driver **ICD00**

■ = Requires the use of Square Driver **PSQD0N**, **PSQD1N** or Driver Tip **RASQ3N**, **RASQ8N**

Description	3.4mm	4.1mm		5mm		6mm
Emergence Profile	3.8	5.0	6.0	5.0	6.0	6.0
Pick-Up Impression Coping	MIC33	IIC12	IIC60	WIP55	WIP56	WIP66
Twist Lock Impression Coping	—	IIC45	IIC46	WIT55	WIT56	WIT66
Laboratory Analog	MMILA	ILA20		ILAW5		ILAW6
Abutment Screw	UNISG*, UNIHG, UNIHT					
Square Try-In Screw (5-pack)	MUNITS	UNITS				
Laboratory Abutment Holder	LTAH5	LTAH7				

*Recommended

Some products may not be available outside of the United States.
 Algunos productos no se comercializan fuera de EE.UU.
 Certains produits ne sont pas disponibles en dehors des États-Unis.
 Einige Produkte sind außerhalb der USA nicht erhältlich.

Screw-Retained Restorations

External Hex Connection

Low Profile Abutments

Indications:

- Single and multi-unit screw-retained restorations
- Minimum interarch space of 7.5mm
- Minimum tissue height of 1mm
- Angle correction up to 30°
- External hex connection 3.4mm(D) Low Profile Abutments are limited for use in the anterior

Material:

Titanium Alloy



3.4mm Seating Surface				
Collar Height	Item Numbers			
	Straight (Non-Hexed)	Straight (Hexed)	17° Pre-Angled (Hexed)	30° Pre-Angled (Hexed)
1mm	LPC341U	LPC341	—	—
2mm	LPC342U	LPC342	LPAC3217	—
3mm	LPC343U	LPC343	—	LPAC3330
4mm	LPC344U	LPC344	LPAC3417	—
5mm	—	—	—	LPAC3530
4.1mm Seating Surface				
Collar Height	Item Numbers			
	Straight (Non-Hexed)	Straight (Hexed)	17° Pre-Angled (Hexed)	30° Pre-Angled (Hexed)
1mm	LPC441U	LPC441	—	—
2mm	LPC442U	LPC442	LPAC4217	—
3mm	LPC443U	LPC443	—	LPAC4330
4mm	LPC444U	LPC444	LPAC4417	—
5mm	—	—	—	LPAC4530
5mm Seating Surface				
Collar Height	Item Numbers			
	Straight (Non-Hexed)	Straight (Hexed)	17° Pre-Angled (Hexed)	30° Pre-Angled (Hexed)
1mm	LPC541U	LPC541	—	—
2mm	LPC542U	LPC542	LPAC5217	—
3mm	LPC543U	LPC543	—	LPAC5330
4mm	LPC544U	LPC544	LPAC5417	—
5mm	—	—	—	LPAC5530











All indicated measurements are in millimeters.

Some products may not be available outside of the United States.
 Algunos productos no se comercializan fuera de EE.UU.
 Certains produits ne sont pas disponibles en dehors des États-Unis.
 Einige Produkte sind außerhalb der USA nicht erhältlich.

Screw-Retained Restorations

External Hex Connection

Low Profile Abutment Components

<i>Pick-Up Impression Coping</i>	<i>Twist Lock™ Impression Coping</i>	<i>Laboratory Analog</i>	<i>Healing Cap</i>	<i>Gold And Castable Cylinder</i>
				
<i>QuickBridge®</i>	<i>Temporary Cylinder</i>	<i>Polishing Protector</i>	<i>Retaining Screw</i>	<i>Driver And Driver Tip</i>
				

◆ = Requires the use of Hex Driver **PHD02N**, **PHD03N** or Driver Tip **RASH3N**, **RASH8N**

○ = Requires the use of Impression Coping Driver **ICD00**

Description		4.8mm Restorative Platform
Pick-Up Impression Coping	hexed > non-hexed >	LPCPIC1 LPCPIC2
Twist Lock Impression Coping	hexed > non-hexed >	LPCTIC1 LPCTIC2
QuickBridge Impression Coping		LPCRIC
Laboratory Analog		LPCLA
Temporary Cylinder	hexed > non-hexed >	LPCTC1 LPCTC2
Healing Cap		LPCHC
PreFormance® Temp. Cylinder	hexed > non-hexed >	LPCPTC1 LPCPTC2
QuickBridge		LPCQB
QuickBridge Replacement Cap		LPCQBCAP
Distal Extension		LPCDE
Gold Cylinder	hexed > non-hexed >	LPCGC1 LPCGC2
Castable Cylinder	hexed > non-hexed >	LPCCC1 LPCCC2
Laser Welded Cylinder		LPCTUCA
Waxing Screw		LPCWS
Retaining Screw		LPCGSH, LPCTSH
Lapping Tool		LPCAMI
Polishing Protector		LPCPP

Abutment Compatibility		
Component	Hexed Abutment	Non-Hexed Abutment
Hexed	Yes	No
Non-Hexed	Yes	Yes

Some products may not be available outside of the United States.
 Algunos productos no se comercializan fuera de EE.UU.
 Certains produits ne sont pas disponibles en dehors des États-Unis.
 Einige Produkte sind außerhalb der USA nicht erhältlich.

Overdenture Restorations

External Hex Connection


LOCATOR® Abutments

Indications:

- Tissue supported removable overdentures on 2-4 implants
- Partially edentulous overdentures with one or more implants
- Limited interarch distance
- Angle correction with up to 40° between divergent implants


Material:

Abutment: Titanium Alloy With Titanium Nitride Coating
 Housing: Titanium Alloy
 Males: Nylon


3.4mm Seating Surface		
Collar Height		Item Numbers
1mm		MLOA001
2mm		MLOA002
3mm		MLOA003
4mm		MLOA004
5mm		MLOA005
6mm		MLOA006





4.1mm Seating Surface		
Collar Height		Item Numbers
1mm		LOA001
2mm		LOA002
3mm		LOA003
4mm		LOA004
5mm		LOA005
6mm		LOA006

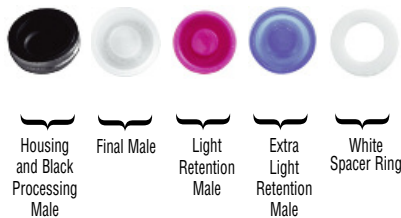

Included With Each Abutment:



Temporary Healing Retention Cylinder
 Retains denture with soft-tissue liner.

	
THRC4 4.1mm(D) x 4mm(H)	THRC6 4.1mm(D) x 6mm(H)


All indicated measurements are in millimeters.

Some products may not be available outside of the United States.
 Algunos productos no se comercializan fuera de EE.UU.
 Certains produits ne sont pas disponibles en dehors des États-Unis.
 Einige Produkte sind außerhalb der USA nicht erhältlich.

Overdenture Restorations

External Hex Connection

LOCATOR® Abutment Components

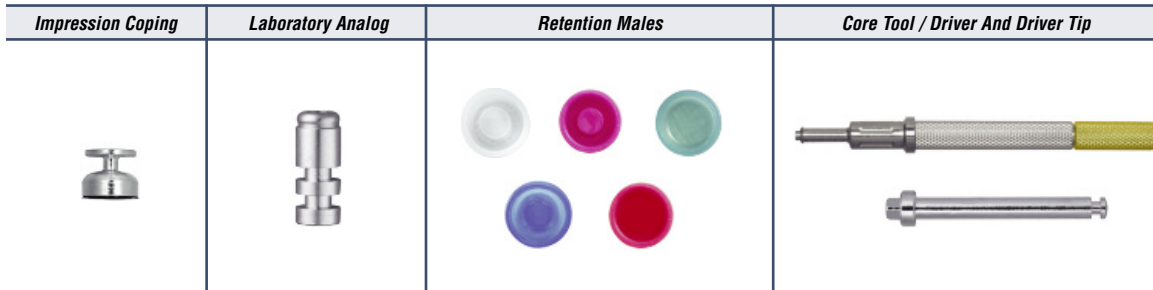

Description	Item Numbers
Impression Coping	LAIC1
Laboratory Analog	LALA1
Extra Light Retention Males (4-pack) - Blue, 1.5lbs/680g	LAELM
Extended Range Males (4-pack) - Green, 4lbs/1800g	LAERM
Extra Light Retention Extended Range Males - Red, 1.5lbs/680g	LELARM
Replacement Males (4-pack) - White, 5lbs/2250g	LARMS
Light Retention Replacement Males (4-pack) - Pink, 3lbs/1350g	LLRMS
Replacement Housing	LOAH
Replacement Housing Kit	LORHK*
Core Tool/Abutment Driver	LCTDR1
Driver Tip 24mm(L)	LOADT4
Driver Tip 30mm(L)	LOADT9
1.25mm/.050in. Driver Tip 24mm(L) - used with LCTDR1	RASH4
1.25mm/.050in. Driver Tip 30mm(L) - used with LCTDR1	RASH9
LOCATOR Bar Attachment	LOAB
LOCATOR Bar Attachment Tap	LOAT
LOCATOR Bar Attachment Drill	LOAD

*Included With **LORHK**
Replacement Housing Kit:




Some products may not be available outside of the United States.
Algunos productos no se comercializan fuera de EE.UU.
Certains produits ne sont pas disponibles en dehors des États-Unis.
Einige Produkte sind außerhalb der USA nicht erhältlich.

Screws


Certain® Internal Connection

Abutment Screws




	<i>Gold-Tite® Screw</i>	<i>Gold-Tite Screw</i>	<i>Titanium Screw</i>	<i>Large Gold-Tite Screw</i>	<i>Large Titanium Screw</i>
Screws	IUNIHG	IZSHG	IUNIHT	ILRGHG	ILRGHT
Drivers	PHD02N, PHD03N	PHD02N, PHD03N	PHD02N, PHD03N	PHD02N, PHD03N	PHD02N, PHD03N
Driver Tips	RASH3N, RASH8N	RASH3N, RASH8N	RASH3N, RASH8N	RASH3N, RASH8N	RASH3N, RASH8N
Torque	20Ncm	20Ncm	20Ncm	20Ncm	20Ncm
For Use With:	UCLA Abutment, GingiHue® Post, GingiHue Post 15°, Hexed Temporary Cylinder, Provide®	ZiReal® Post	UCLA Abutment, GingiHue Post, GingiHue Post 15°, Hexed Temporary Cylinder, Provide	Non-Hexed UCLA Abutment, Non-Hexed Temporary Cylinder, BellaTek® Bars	

Retaining Screws



	<i>Low Profile Abutment Gold-Tite Screw</i>	<i>Gold-Tite Screw</i>	<i>Low Profile Abutment Titanium Screw</i>	<i>Titanium Hexed Screw</i>
Screws	LPCGSH	GSH20, GSH30, GSH70	LPCTSH	TSH30
Drivers	PHD02N, PHD03N	PHD02N, PHD03N	PHD02N, PHD03N	PHD02N, PHD03N
Driver Tips	RASH3N, RASH8N	RASH3N, RASH8N	RASH3N, RASH8N	RASH3N, RASH8N
Torque	10Ncm	10Ncm	10Ncm	10Ncm
For Use With:	Low Profile Abutment	GSH20 - Standard Abutment 6mm(D) X 2mm(H) Conical Abutment 6mm(D) X 1mm(H) GSH30 - Standard, Conical and IOL® Abutments GSH70 - Standard, Conical and IOL Abutments	Low Profile Abutment	Standard, Conical and IOL Abutments

Waxing Screws & Try-In Screws




	<i>Laboratory Waxing Screw</i>	<i>Hexed Try-In Screw (5-pack)</i>
Screws	IWSU30	IUNITS
Drivers	PHD02N, PHD03N	PHD02N, PHD03N
Driver Tips	RASH3N, RASH8N	RASH3N, RASH8N
For Use With:	Pick-Up and Impression Copings, Implant Level Laboratory Procedures	Hexed UCLA Abutment, GingiHue® Post, GingiHue Post 15°, Provide Abutment

Some products may not be available outside of the United States.
 Algunos productos no se comercializan fuera de EE.UU.
 Certains produits ne sont pas disponibles en dehors des États-Unis.
 Einige Produkte sind außerhalb der USA nicht erhältlich.

Screws


External Hex Connection

Abutment Screws




	<i>Gold-Tite® Square</i>	<i>Gold-Tite Hexed</i>	<i>Titanium Hexed</i>
Screws	UNISG	UNIHG	UNIHT
Drivers	PSQD0N, PSQD1N	PHD02N, PHD03N	PHD02N, PHD03N
Driver Tips	RASQ3N, RASQ8N	RASH3N, RASH8N	RASH3N, RASH8N
Torque	32–35Ncm	20Ncm	20Ncm
For Use With:	UCLA Abutment, GingiHue® Post, GingiHue Post 15°, ZiReal® Post, Titanium Cylinder		

Retaining Screws



	<i>Low Profile Abutment Gold-Tite Screw</i>	<i>Gold-Tite Screw</i>	<i>Low Profile Abutment Titanium Screw</i>	<i>Titanium Hexed Screw</i>
Screws	LPCGSH	GSH20, GSH30, GSH70	LPCTSH	TSH30
Drivers	PHD02N, PHD03N	PHD02N, PHD03N	PHD02N, PHD03N	PHD02N, PHD03N
Driver Tips	RASH3N, RASH8N	RASH3N, RASH8N	RASH3N, RASH8N	RASH3N, RASH8N
Torque	10Ncm	10Ncm	10Ncm	10Ncm
For Use With:	Low Profile Abutment	GSH20 - Standard Abutment 6mm(D) X 2mm(H) Conical Abutment 6mm(D) X 1mm(H) GSH30 - Standard, Conical and IOL® Abutments GSH70 - Standard, Conical and IOL Abutments	Low Profile Abutment	Standard, Conical and IOL Abutments

Waxing Screws & Try-In Screws




	<i>Abutment Waxing Screw/Guide Pin</i>	<i>Laboratory Waxing Screw</i>	<i>Square Try-In Screw (5-pack)</i>
Screws	WSK10, WSK15, WSK30	WSU30	UNITS, MUNITS
Drivers	PHD02N, PHD03N	PHD02N, PHD03N	PSQD0N, PSQD1N
Driver Tips	RASH3N, RASH8N	RASH3N, RASH8N	RASQ3N, RASQ8N
For Use With:	Standard and Conical Abutments	Implant Level Laboratory Procedures	UCLA Abutment, GingiHue Post, GingiHue Post 15°, ZiReal Post

Some products may not be available outside of the United States.
 Algunos productos no se comercializan fuera de EE.UU.
 Certains produits ne sont pas disponibles en dehors des États-Unis.
 Einige Produkte sind außerhalb der USA nicht erhältlich.


Miscellaneous Restorative Products

Mechanical Driver Kits

NCATDO *Contra Angle Torque Driver Kit*

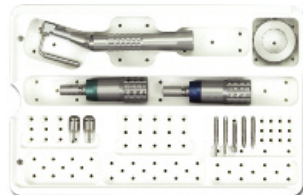

NPSDKO *Prosthetic Driver Kit*

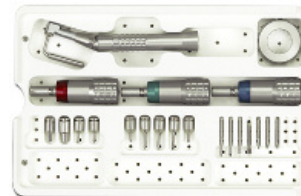

NCATDOC *Contra Angle Torque Driver Kit Certain®*



L-TIRWK *Low Torque Indicating Ratchet Wrench Kit*




NCATDO <i>Contra Angle Torque Kit</i>	NCATDOC <i>Contra Angle Torque Kit Certain</i>	NPSDKO <i>Prosthetic Driver Kit</i>	L-TIRWK <i>Low Torque Indicating Kit</i>	<i>Description</i>	<i>Item Numbers</i>
•	•	•		Narrow Posterior Hex Driver, 17mm(L)	PHD02N
•		•		Narrow Posterior Square Driver, 17mm(L)	PSQD0N
•	•	•		Contra Angle Torque Driver Body	HTD-C
•	•	•	•	Narrow Right Angle Hex Driver Tip, 24mm(L)	RASH3N
•	•	•		Narrow Right Angle Hex Driver Tip, 30mm(L)	RASH8N
•		•	•	Narrow Right Angle Square Driver Tip, 24mm(L)	RASQ3N
•		•		Narrow Right Angle Square Driver Tip, 30mm(L)	RASQ8N
•	•	•		Right Angle Abutment Driver Tip - Steel	RASA3
		•		Contra Angle Torque Controller, 10Ncm	TD-10
•	•	•		Contra Angle Torque Controller, 20Ncm	TD-20
•		•		Contra Angle Torque Controller, 35Ncm	TD-35
•	•	•		Contra Pre-action Handle	CATDH
•	•	•		Prosthetic System Driver Tray	PSDT1
		•		Narrow Impression Coping Driver	ICD00
		•		Posterior Abutment Driver, 17mm(L)	PAD00
		•		Standard Abutment Driver, 24mm(L)	PAD24
		•		Posterior Slotted Screw Driver, 17mm(L)	PSD00
		•		Standard Slotted Screw Driver, 24mm(L)	PSD01
		•		Narrow Standard Slotted Square Driver, 24mm(L)	PSQD1N
		•		Narrow Standard Hex Driver, 24mm(L)	PHD03N
		•		Right Angle Slotted Driver Tip, 24mm(L)	RASD1
		•		Right Angle Slotted Driver Tip, 30mm(L)	RASD6
			•	Low Torque Indicating Ratchet Wrench	L-TIRW
			•	Restorative Torque Tray	RTI2035TR


Some products may not be available outside of the United States.
 Algunos productos no se comercializan fuera de EE.UU.
 Certains produits ne sont pas disponibles en dehors des États-Unis.
 Einige Produkte sind außerhalb der USA nicht erhältlich.

Miscellaneous Restorative Products


Drivers & Driver Tips



Length	Small Hex		Large Hex		Square	
	Driver	Tip	Driver	Tip	Driver	Tip
17mm	PHD00N	—	PHD02N	—	PSQD0N	—
24mm	PHD01N	RASH2N	PHD03N	RASH3N	PSQD1N	RASQ3N
30mm	—	RASH7N	—	RASH8N	—	RASQ8N
For Use With:	External Hex Cover Screws		Healing Abutments, Abutment Screws, Certain® Cover Screws and Retaining Screws		Square Gold-Tite® Abutment Screws and Square Try-in Screws	



Length	Abutment		LOCATOR®
	Driver	Tip	Tip Only
17mm	PAD00	—	—
24mm	PAD24	RASA3	LOADT4
30mm	—	—	LOADT9
For Use With:	Low Profile Abutments		LOCATOR Abutments



Length	Impression Coping	.050" Hex
	Driver Only	Tip Only
17mm	ICD00	—
24mm	—	RASH4
30mm	—	RASH9
For Use With:	Twist Lock™ Transfer Impression Copings	LOCATOR Abutments with LOCATOR Core Tools

MIDT Manual Interchangeable Driver Tip Handle



Some products may not be available outside of the United States.
 Algunos productos no se comercializan fuera de EE.UU.
 Certains produits ne sont pas disponibles en dehors des États-Unis.
 Einige Produkte sind außerhalb der USA nicht erhältlich.

Miscellaneous Restorative Products

Navigator® System Instrumentation Overview



Tapered Navigator Surgical Kit



Tapered Navigator Laboratory Kit



Parallel Walled Navigator Surgical Kit



Parallel Walled Navigator Laboratory Kit

The Navigator System For Guided Surgery

The Navigator System helps clinicians transform computer-based planning into practical implant placement with an opportunity for immediate provisionalization.

The Navigator System features control of hex-orientation to fabricate and deliver provisional restorations immediately following surgery. This unique hex-orientation feature is especially beneficial when immediately loading single tooth cases, cement-retained cases and cases where angulation correction is required.

The Navigator System enables placement and restoration of the following **COMET 3i** Tapered and Parallel Walled Implant Systems:

- Tapered/Parallel Walled Certain® 3.25, 4 and 5mm Implants
- Certain PREVAIL® 3/4/3, 4/3, 4/5/4 and 5/4 Implants
- Certain Tapered PREVAIL 4/3 and 5/4 Implants

An integral part of the Navigator System is the Navigator Laboratory Kit, which contains easy-to-identify components needed to fabricate a master cast and provisional prosthesis prior to the day of surgery. The Navigator Laboratory Kit provides you with the opportunity to:

- Treat patients for immediate-load cases
- Be part of a collaborative approach to comprehensive patient treatment
- Embrace emerging technology with open architecture compatibility that provides freedom to choose among leading planning software solutions

Miscellaneous Restorative Products


Tapered Navigator® Laboratory Kit

SGTLKIT Tapered Navigator Laboratory Kit

For Certain® Tapered Implants Including:

- Certain 3.25, 4 and 5mm Implants
- Certain Tapered PREVAIL® 4/3 and 5/4 Implants




	Description	Item Numbers
•	Tapered Navigator Laboratory Tray	SGTLTRAY
•	Navigator Certain Analog Mount, 3.4mm(D) - Short	MSGIAMS
•	Navigator Certain Analog Mount, 3.4mm(D) - Long	MSGIAML
•	Navigator Certain Analog Mount, 4.1mm(D) - Short	SGIAM4S
•	Navigator Certain Analog Mount, 4.1mm(D) - Long	SGIAM4L
•	Navigator Certain Analog Mount, 5mm(D) - Short	SGIAM5S
•	Navigator Certain Analog Mount, 5mm(D) - Long	SGIAM5L


Parallel Walled Navigator Laboratory Kit

SGLKIT Navigator Laboratory Kit

For Certain Parallel Walled Implants Including:

- Certain 3.25, 4 and 5mm Implants
- Certain Tapered PREVAIL 4/3 and 5/4 Implants



	Description	Item Numbers
•	Navigator Laboratory Tray	SGLTRAY
•	Navigator Certain Analog Mount, 3.4mm(D) x 1(L)	MSGIAM1
•	Navigator Certain Analog Mount, 3.4mm(D) x 2(L)	MSGIAM2
•	Navigator Certain Analog Mount, 3.4mm(D) x 3(L)	MSGIAM3
•	Navigator Certain Analog Mount, 3.4mm(D) x 4(L)	MSGIAM4
•	Navigator Certain Analog Mount, 4.1mm(D) x 1(L)	SGIAM41
•	Navigator Certain Analog Mount, 4.1mm(D) x 2(L)	SGIAM42
•	Navigator Certain Analog Mount, 4.1mm(D) x 3(L)	SGIAM43
•	Navigator Certain Analog Mount, 4.1mm(D) x 4(L)	SGIAM44
•	Navigator Certain Analog Mount, 5mm(D) x 1(L)	SGIAM51
•	Navigator Certain Analog Mount, 5mm(D) x 2(L)	SGIAM52
•	Navigator Certain Analog Mount, 5mm(D) x 3(L)	SGIAM53
•	Navigator Certain Analog Mount, 5mm(D) x 4(L)	SGIAM54

Some products may not be available outside of the United States.
 Algunos productos no se comercializan fuera de EE.UU.
 Certains produits ne sont pas disponibles en dehors des États-Unis.
 Einige Produkte sind außerhalb der USA nicht erhältlich.

Miscellaneous Restorative Products

Laboratory Tools

Lapping Tool For Castable UCLA Abutment With Guide



RH600 Reamer With Handle




IQSA01 Certain QuickSeat® Activator Tool



Polishing Protector, UCLA Abutment



Laboratory Abutment Holder

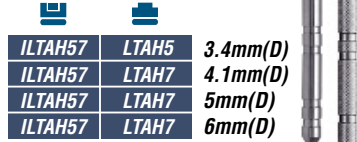

Miscellaneous Items

L-TIRW Low Torque Indicating Ratchet Wrench

L-TIRWK Low Torque Indicating Ratchet Wrench Kit

C9980


Standard ISO 1797 Adapter

C9981


Short ISO 1797 Adapter




AG900 Prosthetic Angle Guide Kit




TMP80 Tissue Measuring Post



ISRT10 Certain Screw Removal Kit

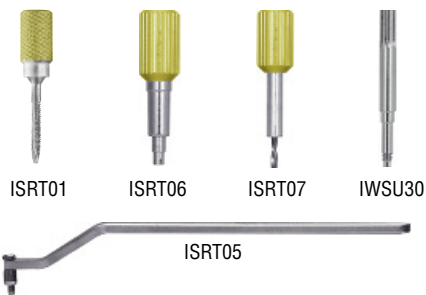

SRT10 Screw Removal Kit

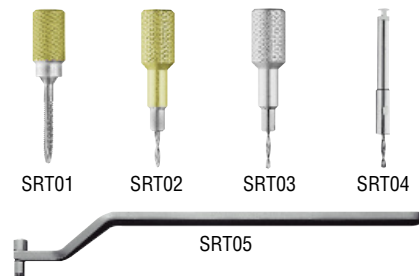

All indicated measurements are in millimeters.

Some products may not be available outside of the United States.
 Algunos productos no se comercializan fuera de EE.UU.
 Certains produits ne sont pas disponibles en dehors des États-Unis.
 Einige Produkte sind außerhalb der USA nicht erhältlich.

Patient Education Products

Description	Item Numbers
Patient Ed Model - DIEM®2 (4-unit)	DIEM2-4UNIT
Patient Ed Model - DIEM 2 (6-unit)	DIEM2-6UNIT
Patient Ed Model - OSSEOTITE® Implant	EXHEXMOD
Patient Ed Model - LOCATOR®	PEMODLOC
Patient Ed Model - Single/Multiple Teeth	PEMODSM
Patient Ed Brochure - Bone Loss (25-pack)	ART885
Patient Ed Brochure - Multiple Teeth (25-pack)	ART887
Patient Ed Brochure - Implant Retained, Fixed (25-pack)	ART888
Patient Ed Brochure - Implant Retained, LOCATOR (25-pack)	ART889
Patient Ed Brochure - Implant Retained, Bar (25-pack)	ART890
Patient Ed Brochure - Immediate Teeth Replacement, DIEM (25-pack)	ART929
Patient Ed Care Card (25-pack)	ART930
Patient Ed Flip Chart	ART943
Patient Ed DVD - Multilingual Version	ART951EUR
Patient Ed Brochure - Bone Loss (Spanish Version)	ART957S
Patient Ed Awareness and Education Poster	ART962
Patient Ed Quad-fold Brochure with Holder (25-pack)	ART1154
Patient Ed General Brochure (25-pack)	ART1157
Patient Ed Regenerative Brochure	ART1178



Some products may not be available outside of the United States.
 Algunos productos no se comercializan fuera de EE.UU.
 Certains produits ne sont pas disponibles en dehors des États-Unis.
 Einige Produkte sind außerhalb der USA nicht erhältlich.

Index

Cat. #	Description	Page#	Cat. #	Description	Page#
AG900	PROSTHETIC ANGLE GUIDE KIT (9-PIECE SET)	33	IILAW5	CERTAIN IMPLANT LAB ANALOG 5MM(D)	4,6,10
APP452G	GINGIHUE® POST 4.1MM(D) X 5MM(P) X 2MM(H)	17	IILAW6	CERTAIN IMPLANT LAB ANALOG 6MM(D)	4,6,10
APP454G	GINGIHUE POST 4.1MM(D) X 5MM(P) X 4MM(H)	17	IITCS41	CERTAIN TEMPORARY (HEXED) CYLINDER 4.1MM(D) W/HEXED SCREW	2
APP462G	GINGIHUE POST 4.1MM(D) X 6MM(P) X 2MM(H)	17	IITCS42	CERTAIN TEMPORARY (NON-HEXED) CYLINDER 4.1MM(D) W/LARGE DIA. SCREW	2
APP464G	GINGIHUE POST 4.1MM(D) X 6MM(P) X 4MM(H)	17	ILA20	IMPLANT LAB ANALOG 4.1MM(D)	18,20,22
ART1178	PATIENT ED REGENERATIVE BROCHURE	34	ILAW5	IMPLANT LAB ANALOG 5MM(D)	18,20,22
ART885	PATIENT ED BROCHURE - BONE LOSS (25-PACK)	34	ILAW6	IMPLANT LAB ANALOG 6MM(D)	18,20,22
ART887	PATIENT ED BROCHURE - MULTIPLE TEETH (25-PACK)	34	ILOA001	CERTAIN LOCATOR ABUTMENT 4.1MM(D) X 1MM(H)	13
ART888	PATIENT ED BROCHURE - IMPLANT RETAINED, FIXED (25-PACK)	34	ILOA002	CERTAIN LOCATOR ABUTMENT 4.1MM(D) X 2MM(H)	13
ART889	PATIENT ED BROCHURE - IMPLANT RETAINED, LOCATOR® (25-PACK)	34	ILOA003	CERTAIN LOCATOR ABUTMENT 4.1MM(D) X 3MM(H)	13
ART890	PATIENT ED BROCHURE - IMPLANT RETAINED, BAR (25-PACK)	34	ILOA004	CERTAIN LOCATOR ABUTMENT 4.1MM(D) X 4MM(H)	13
ART929	PATIENT ED BROCHURE - IMMEDIATE TEETH REPLACEMENT, DIEM® (25-PACK)	34	ILOA005	CERTAIN LOCATOR ABUTMENT 4.1MM(D) X 5MM(H)	13
ART930	PATIENT ED CARE CARD (25-PACK)	34	ILOA006	CERTAIN LOCATOR ABUTMENT 4.1MM(D) X 6MM(H)	13
ART943	PATIENT ED FLIP CHART	34	ILPAC3217	CERTAIN LOW PROFILE 17° PRE-ANGLED ABUTMENT 3.4MM(D) X 2MM(H)	11
ART951EUR	PATIENT ED DVD - MULTILINGUAL VERSION	34	ILPAC3330	CERTAIN LOW PROFILE 30° PRE-ANGLED ABUTMENT 3.4MM(D) X 3MM(H)	11
ART957S	PATIENT ED BROCHURE - BONE LOSS (SPANISH VERSION)	34	ILPAC3417	CERTAIN LOW PROFILE 17° PRE-ANGLED ABUTMENT 3.4MM(D) X 4MM(H)	11
ART962	PATIENT ED AWARENESS AND EDUCATION POSTER	34	ILPAC3530	CERTAIN LOW PROFILE 30° PRE-ANGLED ABUTMENT 3.4MM(D) X 5MM(H)	11
C9980	LOW TORQUE INDICATING RATCHET WRENCH STANDARD ISO 1797 ADAPTER	33	ILPAC4217	CERTAIN LOW PROFILE 17° PRE-ANGLED ABUTMENT 4.1MM(D) X 2MM(H)	11
C9981	LOW TORQUE INDICATING RATCHET WRENCH SHORT ISO 1797 ADAPTER	33	ILPAC4330	CERTAIN LOW PROFILE 30° PRE-ANGLED ABUTMENT 4.1MM(D) X 3MM(H)	11
CAP454	ZIREAL® POST 4.1MM(D) X 5MM(P) X 4MM(H)	17	ILPAC4417	CERTAIN LOW PROFILE 17° PRE-ANGLED ABUTMENT 4.1MM(D) X 4MM(H)	11
CAP464	ZIREAL POST 4.1MM(D) X 6MM(P) X 4MM(H)	17	ILPAC4530	CERTAIN LOW PROFILE 30° PRE-ANGLED ABUTMENT 4.1MM(D) X 5MM(H)	11
CATDH	CONTRA ANGLE TORQUE DRIVER HANDLE	29	ILPAC5217	CERTAIN LOW PROFILE 17° PRE-ANGLED ABUTMENT 5MM(D) X 2MM(H)	11
DIEM2-4UNIT	PATIENT ED MODEL - DIEM 2 (4-UNIT)	34	ILPAC5330	CERTAIN LOW PROFILE 30° PRE-ANGLED ABUTMENT 5MM(D) X 3MM(H)	11
DIEM2-6UNIT	PATIENT ED MODEL - DIEM 2 (6-UNIT)	34	ILPAC5417	CERTAIN LOW PROFILE 17° PRE-ANGLED ABUTMENT 5MM(D) X 4MM(H)	11
EXHEXMOD	PATIENT ED MODEL - OSSEOTITE® IMPLANT	34	ILPAC5530	CERTAIN LOW PROFILE 30° PRE-ANGLED ABUTMENT 5MM(D) X 5MM(H)	11
GSH20	GOLD-TITE® (HEXED) RETAINING SCREW 2MM	27,28	ILPC341	CERTAIN LOW PROFILE TWO-PIECE ABUTMENT 3.4MM(D) X 1MM(H)	11
GSH30	GOLD-TITE (HEXED) RETAINING SCREW 3MM	27,28	ILPC341U	CERTAIN LOW PROFILE ONE-PIECE ABUTMENT 3.4MM(D) X 1MM(H)	11
GSH70	GOLD-TITE (HEXED) RETAINING SCREW 7MM	27,28	ILPC342	CERTAIN LOW PROFILE TWO-PIECE ABUTMENT 3.4MM(D) X 2MM(H)	11
GUCA1C	UCLA GOLD (HEXED) ABUTMENT CYLINDER 4.1MM(D)	19,21	ILPC342U	CERTAIN LOW PROFILE ONE-PIECE ABUTMENT 3.4MM(D) X 2MM(H)	11
GUCA2C	UCLA GOLD (NON-HEXED) ABUTMENT CYLINDER 4.1MM(D)	21	ILPC343	CERTAIN LOW PROFILE TWO-PIECE ABUTMENT 3.4MM(D) X 3MM(H)	11
HTD-C	CONTRA ANGLE TORQUE DRIVER BODY	29	ILPC343U	CERTAIN LOW PROFILE ONE-PIECE ABUTMENT 3.4MM(D) X 3MM(H)	11
IAPP452G	CERTAIN® GINGIHUE POST 4.1MM(D) X 5MM(P) X 2MM(H)	3	ILPC344	CERTAIN LOW PROFILE TWO-PIECE ABUTMENT 3.4MM(D) X 4MM(H)	11
IAPP454G	CERTAIN GINGIHUE POST 4.1MM(D) X 5MM(P) X 4MM(H)	3	ILPC344U	CERTAIN LOW PROFILE ONE-PIECE ABUTMENT 3.4MM(D) X 4MM(H)	11
IAPP462G	CERTAIN GINGIHUE POST 4.1MM(D) X 6MM(P) X 2MM(H)	3	ILPC441	CERTAIN LOW PROFILE TWO-PIECE ABUTMENT 4.1MM(D) X 1MM(H)	11
IAPP464G	CERTAIN GINGIHUE POST 4.1MM(D) X 6MM(P) X 4MM(H)	3	ILPC441U	CERTAIN LOW PROFILE ONE-PIECE ABUTMENT 4.1MM(D) X 1MM(H)	11
IAPP472G	CERTAIN GINGIHUE POST 4.1MM(D) X 7.5MM(P) X 2MM(H)	3	ILPC442	CERTAIN LOW PROFILE TWO-PIECE ABUTMENT 4.1MM(D) X 2MM(H)	11
IAPP474G	CERTAIN GINGIHUE POST 4.1MM(D) X 7.5MM(P) X 4MM(H)	3	ILPC442U	CERTAIN LOW PROFILE ONE-PIECE ABUTMENT 4.1MM(D) X 2MM(H)	11
ICD00	NARROW IMPRESSION COPING DRIVER	29,30	ILPC443	CERTAIN LOW PROFILE TWO-PIECE ABUTMENT 4.1MM(D) X 3MM(H)	11
IGUCA1C	CERTAIN UCLA GOLD (HEXED) ABUTMENT CYLINDER 4.1MM(D)	5,9	ILPC443U	CERTAIN LOW PROFILE ONE-PIECE ABUTMENT 4.1MM(D) X 3MM(H)	11
IGUCA2C	CERTAIN UCLA GOLD (NON-HEXED) ABUTMENT CYLINDER 4.1MM(D)	9	ILPC444	CERTAIN LOW PROFILE TWO-PIECE ABUTMENT 4.1MM(D) X 4MM(H)	11
IGUCA2T	CERTAIN UCLA GOLD (NON-HEXED) ABUTMENT CYLINDER 4.1MM(D) W/LARGE DIAMETER TITANIUM SCREW	9	ILPC444U	CERTAIN LOW PROFILE ONE-PIECE ABUTMENT 4.1MM(D) X 4MM(H)	11
IIC12	IMPLANT EP® PICK-UP COPING 4.1MM(D) X 5MM(P)	18,20,22	ILPC541	CERTAIN LOW PROFILE TWO-PIECE ABUTMENT 5MM(D) X 1MM(H)	11
IIC45	IMPLANT EP TWIST LOCK™ COPING 4.1MM(D) X 5MM(P)	18,20,22	ILPC541U	CERTAIN LOW PROFILE ONE-PIECE ABUTMENT 5MM(D) X 1MM(H)	11
IIC46	IMPLANT EP TWIST LOCK COPING 4.1MM(D) X 6MM(P)	18,20,22	ILPC542	CERTAIN LOW PROFILE TWO-PIECE ABUTMENT 5MM(D) X 2MM(H)	11
IIC60	IMPLANT EP PICK-UP COPING 4.1MM(D) X 6MM(P)	18,20,22	ILPC542U	CERTAIN LOW PROFILE ONE-PIECE ABUTMENT 5MM(D) X 2MM(H)	11
IIC12	CERTAIN EP PICK-UP COPING 4.1MM(D) X 5MM(P)	4,6,10	ILPC543	CERTAIN LOW PROFILE TWO-PIECE ABUTMENT 5MM(D) X 3MM(H)	11
IIC41	CERTAIN STRAIGHT PICK-UP COPING 4.1MM(D) X 4.1MM(P)	4,6,10	ILPC543U	CERTAIN LOW PROFILE ONE-PIECE ABUTMENT 5MM(D) X 3MM(H)	11
IIC42	CERTAIN EP PICK-UP COPING 4.1MM(D) X 4.1MM(P)	4,6,10	ILPC544	CERTAIN LOW PROFILE TWO-PIECE ABUTMENT 5MM(D) X 4MM(H)	11
IIC44	CERTAIN STRAIGHT TWIST LOCK COPING 4.1MM(D) X 4.1MM(P)	4,6,10	ILPC544U	CERTAIN LOW PROFILE ONE-PIECE ABUTMENT 5MM(D) X 4MM(H)	11
IIC45	CERTAIN EP TWIST LOCK COPING 4.1MM(D) X 5MM(P)	4,6,10	ILRGHG	CERTAIN GOLD-TITE (HEXED) LARGE SCREW	10,27
IIC46	CERTAIN EP TWIST LOCK COPING 4.1MM(D) X 6MM(P)	4,6,10	ILRGHT	CERTAIN TITANIUM (HEXED) LARGE SCREW	10,27
IIC60	CERTAIN EP PICK-UP COPING 4.1MM(D) X 6MM(P)	4,6,10	ILT150	CERTAIN LAPPING TOOL FOR CASTABLE UCLA ABUTMENT W/GUIDE 4MM(D)	33
IILA20	CERTAIN IMPLANT LAB ANALOG 4.1MM(D)	4,6,10	ILTAH57	CERTAIN LABORATORY ABUTMENT HOLDER FOR ALL CERTAIN PLATFORMS	4,6,10,33

Index

Cat. #	Description	Page#	Cat. #	Description	Page#
IMAP32G	CERTAIN® GINGIHUE® POST 3.4MM(D) X 3.8MM(P) X 2MM(H)	3	IPA5255	PROVIDE ABUTMENT - 5MM(PLATFORM) X 2MM(COLLAR) X 5.5MM(POST) X 6.5MM(PROFILE)	7
IMAP34G	CERTAIN GINGIHUE POST 3.4MM(D) X 3.8MM(P) X 4MM(H)	3	IPA5340	PROVIDE ABUTMENT - 5MM(PLATFORM) X 3MM(COLLAR) X 4MM(POST) X 6.5MM(PROFILE)	7
IMIC30	CERTAIN EP® PICK-UP COPING 3.4MM(D) X 3.4MM(P)	4,6,10	IPA5355	PROVIDE ABUTMENT - 5MM(PLATFORM) X 3MM(COLLAR) X 5.5MM(POST) X 6.5MM(PROFILE)	7
IMIC33	CERTAIN EP PICK-UP COPING 3.4MM(D) X 3.8MM(P)	4,6,10	IPA5440	PROVIDE ABUTMENT - 5MM(PLATFORM) X 4MM(COLLAR) X 4MM(POST) X 6.5MM(PROFILE)	7
IMIC35	CERTAIN EP PICK-UP COPING 3.4MM(D) X 5MM(P)	4,6,10	IPA5455	PROVIDE ABUTMENT - 5MM(PLATFORM) X 4MM(COLLAR) X 5.5MM(POST) X 6.5MM(PROFILE)	7
IMIT33	CERTAIN EP TWIST LOCK COPING 3.4MM(D) X 3.8MM(P)	4,6,10	IPA6140	PROVIDE ABUTMENT - 6MM(PLATFORM) X 1MM(COLLAR) X 4MM(POST) X 6.5MM(PROFILE)	7
IMIT35	CERTAIN EP TWIST LOCK COPING 3.4MM(D) X 5MM(P)	4,6,10	IPA6155	PROVIDE ABUTMENT - 6MM(PLATFORM) X 1MM(COLLAR) X 5.5MM(POST) X 6.5MM(PROFILE)	7
IMLOA001	CERTAIN LOCATOR® ABUTMENT 3.4MM(D) X 1MM(H)	13	IPA6240	PROVIDE ABUTMENT - 6MM(PLATFORM) X 2MM(COLLAR) X 4MM(POST) X 6.5MM(PROFILE)	7
IMLOA002	CERTAIN LOCATOR ABUTMENT 3.4MM(D) X 2MM(H)	13	IPA6255	PROVIDE ABUTMENT - 6MM(PLATFORM) X 2MM(COLLAR) X 5.5MM(POST) X 6.5MM(PROFILE)	7
IMLOA003	CERTAIN LOCATOR ABUTMENT 3.4MM(D) X 3MM(H)	13	IPA6340	PROVIDE ABUTMENT - 6MM(PLATFORM) X 3MM(COLLAR) X 4MM(POST) X 6.5MM(PROFILE)	7
IMLOA004	CERTAIN LOCATOR ABUTMENT 3.4MM(D) X 4MM(H)	13	IPA6355	PROVIDE ABUTMENT - 6MM(PLATFORM) X 3MM(COLLAR) X 5.5MM(POST) X 6.5MM(PROFILE)	7
IMLOA005	CERTAIN LOCATOR ABUTMENT 3.4MM(D) X 5MM(H)	13	IPA6440	PROVIDE ABUTMENT - 6MM(PLATFORM) X 4MM(COLLAR) X 4MM(POST) X 6.5MM(PROFILE)	7
IMLOA006	CERTAIN LOCATOR ABUTMENT 3.4MM(D) X 6MM(H)	13	IPA6455	PROVIDE ABUTMENT - 6MM(PLATFORM) X 4MM(COLLAR) X 5.5MM(POST) X 6.5MM(PROFILE)	7
IMLT150	CERTAIN LAPPING TOOL FOR CASTABLE UCLA ABUTMENT W/GUIDE 3.4MM(D)	33	IPAP452G	CERTAIN GINGIHUE 15° PRE-ANGLED POST 4.1MM(D) X 5MM(P) X 2MM(H)	3
IMMILA	CERTAIN IMPLANT LAB ANALOG 3.4MM(D)	4,6,10	IPAP454G	CERTAIN GINGIHUE 15° PRE-ANGLED POST 4.1MM(D) X 5MM(P) X 4MM(H)	3
IMMTC51	CERTAIN TEMPORARY HEXED CYLINDER 3.4MM(D) W/HEXED SCREW	2	IPAP462G	CERTAIN GINGIHUE 15° PRE-ANGLED POST 4.1MM(D) X 6MM(P) X 2MM(H)	3
IMPAP32G	CERTAIN GINGIHUE 15° PRE-ANGLED POST 3.4MM(D) X 3.8MM(P) X 2MM(H)	3	IPAP464G	CERTAIN GINGIHUE 15° PRE-ANGLED POST 4.1MM(D) X 6MM(P) X 4MM(H)	3
IMPAP34G	CERTAIN GINGIHUE 15° PRE-ANGLED POST 3.4MM(D) X 3.8MM(P) X 4MM(H)	3	IPAP472G	CERTAIN GINGIHUE 15° PRE-ANGLED POST 4.1MM(D) X 7.5MM(P) X 2MM(H)	3
IMPAPF34	CERTAIN PREFORMANCE® 15° PRE-ANGLED POST 3.4MM(D) X 3.8MM(P) X 4MM(H)	1	IPAP474G	CERTAIN GINGIHUE 15° PRE-ANGLED POST 4.1MM(D) X 7.5MM(P) X 4MM(H)	3
IMPAPF36	CERTAIN PREFORMANCE 15° PRE-ANGLED POST 3.4MM(D) X 3.8MM(P) X 6MM(H)	1	IPAP552G	CERTAIN GINGIHUE 15° PRE-ANGLED POST 5MM(D) X 5MM(P) X 2MM(H)	3
IMPPF34	CERTAIN PREFORMANCE POST 3.4MM(D) X 3.8MM(P) X 4MM(H)	1	IPAP554G	CERTAIN GINGIHUE 15° PRE-ANGLED POST 5MM(D) X 5MM(P) X 4MM(H)	3
IMPPF36	CERTAIN PREFORMANCE POST 3.4MM(D) X 3.8MM(P) X 6MM(H)	1	IPAP562G	CERTAIN GINGIHUE 15° PRE-ANGLED POST 5MM(D) X 6MM(P) X 2MM(H)	3
IMPFTC32	CERTAIN PREFORMANCE (NON-HEXED) TEMPORARY CYLINDER 3.4MM(D)	2	IPAP564G	CERTAIN GINGIHUE 15° PRE-ANGLED POST 5MM(D) X 6MM(P) X 4MM(H)	3
IMPFTC34	CERTAIN PREFORMANCE (HEXED) TEMPORARY CYLINDER 3.4MM(D)	2	IPAP572G	CERTAIN GINGIHUE 15° PRE-ANGLED POST 5MM(D) X 7.5MM(P) X 2MM(H)	3
IMUCC2C	CERTAIN UCLA CASTABLE (NON-HEXED) ABUTMENT CYLINDER 3.4MM(D)	9	IPAP574G	CERTAIN GINGIHUE 15° PRE-ANGLED POST 5MM(D) X 7.5MM(P) X 4MM(H)	3
IMUCC2T	CERTAIN UCLA CASTABLE (NON-HEXED) ABUTMENT CYLINDER 3.4MM(D) W/LARGE DIAMETER TITANIUM SCREW	9	IPAP662G	CERTAIN GINGIHUE 15° PRE-ANGLED POST 6MM(D) X 6MM(P) X 2MM(H)	3
IMUCG1C	CERTAIN UCLA GOLD (HEXED) ABUTMENT CYLINDER 3.4MM(D)	5,9	IPAP664G	CERTAIN GINGIHUE 15° PRE-ANGLED POST 6MM(D) X 6MM(P) X 4MM(H)	3
IMUCG2C	CERTAIN UCLA GOLD (NON-HEXED) ABUTMENT CYLINDER 3.4MM(D)	9	IPAP672G	CERTAIN GINGIHUE 15° PRE-ANGLED POST 6MM(D) X 7.5MM(P) X 2MM(H)	3
IMUCG2T	CERTAIN UCLA GOLD (NON-HEXED) ABUTMENT CYLINDER 3.4MM(D) W/LARGE DIAMETER TITANIUM SCREW	9	IPAP674G	CERTAIN GINGIHUE 15° PRE-ANGLED POST 6MM(D) X 7.5MM(P) X 4MM(H)	3
IPA4140	PROVIDE® ABUTMENT - 4.1MM(PLATFORM) X 1MM(COLLAR) X 4MM(POST) X 4.8MM(PROFILE)	7	IPAPF454	CERTAIN PREFORMANCE 15° PRE-ANGLED POST 4.1MM(D) X 5MM(P) X 4MM(H)	1
IPA4155	PROVIDE ABUTMENT - 4.1MM(PLATFORM) X 1MM(COLLAR) X 5.5MM(POST) X 4.8MM(PROFILE)	7	IPAPF456	CERTAIN PREFORMANCE 15° PRE-ANGLED POST 4.1MM(D) X 5MM(P) X 6MM(H)	1
IPA4240	PROVIDE ABUTMENT - 4.1MM(PLATFORM) X 2MM(COLLAR) X 4MM(POST) X 4.8MM(PROFILE)	7	IPAPF554	CERTAIN PREFORMANCE 15° PRE-ANGLED POST 5MM(D) X 5MM(P) X 4MM(H)	1
IPA4255	PROVIDE ABUTMENT - 4.1MM(PLATFORM) X 2MM(COLLAR) X 5.5MM(POST) X 4.8MM(PROFILE)	7			
IPA4340	PROVIDE ABUTMENT - 4.1MM(PLATFORM) X 3MM(COLLAR) X 4MM(POST) X 4.8MM(PROFILE)	7			
IPA4355	PROVIDE ABUTMENT - 4.1MM(PLATFORM) X 3MM(COLLAR) X 5.5MM(POST) X 4.8MM(PROFILE)	7			
IPA4440	PROVIDE ABUTMENT - 4.1MM(PLATFORM) X 4MM(COLLAR) X 4MM(POST) X 4.8MM(PROFILE)	7			
IPA4455	PROVIDE ABUTMENT - 4.1MM(PLATFORM) X 4MM(COLLAR) X 5.5MM(POST) X 4.8MM(PROFILE)	7			
IPA5140	PROVIDE ABUTMENT - 5MM(PLATFORM) X 1MM(COLLAR) X 4MM(POST) X 6.5MM(PROFILE)	7			
IPA5155	PROVIDE ABUTMENT - 5MM(PLATFORM) X 1MM(COLLAR) X 5.5MM(POST) X 6.5MM(PROFILE)	7			
IPA5240	PROVIDE ABUTMENT - 5MM(PLATFORM) X 2MM(COLLAR) X 4MM(POST) X 6.5MM(PROFILE)	7			

Index

Cat.#	Description	Page#	Cat.#	Description	Page#
IPAPF556	CERTAIN® PERFORMANCE® 15° PRE-ANGLED POST 5MM(D) X 5MM(P) X 6MM(H)	1	IWPFTC52	CERTAIN PERFORMANCE (NON-HEXED) TEMPORARY CYLINDER 5MM(D) 2	
IPAPF664	CERTAIN PERFORMANCE 15° PRE-ANGLED POST 6MM(D) X 6MM(P) X 4MM(H)	1	IWPFTC61	CERTAIN PERFORMANCE (HEXED) TEMPORARY CYLINDER 6MM(D)	2
IPAPF666	CERTAIN PERFORMANCE 15° PRE-ANGLED POST 6MM(D) X 6MM(P) X 6MM(H)	1	IWPFTC62	CERTAIN PERFORMANCE (NON-HEXED) TEMPORARY CYLINDER 6MM(D)	2
IPFP454	CERTAIN PERFORMANCE POST 4.1MM(D) X 5MM(P) X 4MM(H)	1	IWPP552G	CERTAIN GINGIHUE® POST 5MM(D) X 5MM(P) X 2MM(H)	3
IPFP456	CERTAIN PERFORMANCE POST 4.1MM(D) X 5MM(P) X 6MM(H)	1	IWPP554G	CERTAIN GINGIHUE POST 5MM(D) X 5MM(P) X 4MM(H)	3
IPFTC41	CERTAIN PERFORMANCE (HEXED) TEMPORARY CYLINDER 4.1MM(D)	2	IWPP562G	CERTAIN GINGIHUE POST 5MM(D) X 6MM(P) X 2MM(H)	3
IPFTC42	CERTAIN PERFORMANCE (NON-HEXED) TEMPORARY CYLINDER 4.1MM(D)	2	IWPP564G	CERTAIN GINGIHUE POST 5MM(D) X 6MM(P) X 4MM(H)	3
IPPIA3	CERTAIN UCLA POLISHING PROTECTOR 4.1MM(D)	33	IWPP572G	CERTAIN GINGIHUE POST 5MM(D) X 7.5MM(P) X 2MM(H)	3
IPPIA5	CERTAIN UCLA POLISHING PROTECTOR 5MM(D)	33	IWPP574G	CERTAIN GINGIHUE POST 5MM(D) X 7.5MM(P) X 4MM(H)	3
IPPIA6	CERTAIN UCLA POLISHING PROTECTOR 6MM(D)	33	IWPP662G	CERTAIN GINGIHUE POST 6MM(D) X 6MM(P) X 2MM(H)	3
IPPM1	CERTAIN UCLA POLISHING PROTECTOR 3.4MM(D)	33	IWPP664G	CERTAIN GINGIHUE POST 6MM(D) X 6MM(P) X 4MM(H)	3
IQSA01	CERTAIN QUICKSEAT® ACTIVATOR TOOL	9,33	IWPP672G	CERTAIN GINGIHUE POST 6MM(D) X 7.5MM(P) X 2MM(H)	3
IRH600	CERTAIN REAMER WITH HANDLE	33	IWPP674G	CERTAIN GINGIHUE POST 6MM(D) X 7.5MM(P) X 4MM(H)	3
ISRT01	CERTAIN HAND TAP	33	IWSU30	CERTAIN WAXING SCREW W/GUIDE PIN	27,33
ISRT05	CERTAIN GUIDE HANDLE	33	IWTCS51	CERTAIN TEMPORARY (HEXED) CYLINDER 5MM(D) W/HEXED SCREW	2
ISRT06	CERTAIN SCREW REMOVAL TOOL	33	IWTCS52	CERTAIN TEMPORARY (NON-HEXED) CYLINDER 5MM(D) W/LARGE DIA. SCREW	2
ISRT07	MANUAL REVERSING TOOL	33	IWTCS61	CERTAIN TEMPORARY (HEXED) CYLINDER 6MM(D) W/HEXED SCREW	2
ISRT10	CERTAIN SCREW REMOVAL KIT	33	IWTCS62	CERTAIN TEMPORARY (NON-HEXED) CYLINDER 6MM(D) W/LARGE DIA. SCREW	2
ITCS41	TEMPORARY (HEXED) IMPLANT CYLINDER 4.1MM(D)	16	IZIRTS	CERTAIN ZIRCONIA TRY-IN (HEXED) SCREW	4
ITCS42	TEMPORARY (NON-HEXED) IMPLANT CYLINDER 4.1MM(D)	16	IZSHG	CERTAIN ZIREAL® GOLD-TITE (HEXED) SCREW	4,27
IUNAB2C	CERTAIN UCLA CASTABLE (NON-HEXED) ABUTMENT CYLINDER 4.1MM(D)	9	LAELM	LOCATOR® EXTRA LIGHT RETENTION MALES (4-PACK)	14,26
IUNAB2T	CERTAIN UCLA CASTABLE (NON-HEXED) ABUTMENT CYLINDER 4.1MM(D) 9 W/LARGE DIAMETER TITANIUM SCREW	9	LAERM	LOCATOR EXTENDED RANGE MALES - GREEN, 4LBS/1800G (4-PACK)	14,26
IUNIHG	CERTAIN GOLD-TITE® (HEXED) SCREW	4,6,8,10,27	LAIC1	LOCATOR ABUTMENT IMPRESSION COPING	14,26
IUNIHT	CERTAIN TITANIUM (HEXED) SCREW	4,6,8,10,27	LALA1	LOCATOR ABUTMENT LAB ANALOG	14,26
IUNITS	CERTAIN TRY-IN (HEXED) SCREW (5-PACK) 3.4, 4.1, 5, 6MM(D)	4,6,10,27	LARMS	LOCATOR REPLACEMENT MALES - WHITE, 5LBS/2250G (4-PACK)	14,26
IWGA51C	CERTAIN UCLA GOLD (HEXED) ABUTMENT CYLINDER 5MM(D)	5,9	LCTDR1	LOCATOR CORE TOOL/ABUTMENT DRIVER	14,26
IWGA52C	CERTAIN UCLA GOLD (NON-HEXED) ABUTMENT CYLINDER 5MM(D)	9	LELARM	EXTRA LIGHT RETENTION EXTENDED RANGE MALES - RED, 1.5LBS/680G	14,26
IWGA52T	CERTAIN UCLA GOLD (NON-HEXED) ABUTMENT CYLINDER 5MM(D) W/LARGE DIAMETER TITANIUM SCREW	9	LLRMS	LOCATOR LIGHT RETENTION REPLACEMENT MALES - PINK, 3LBS/1350G (4-PACK)	14,26
IWGA61C	CERTAIN UCLA GOLD (HEXED) ABUTMENT CYLINDER 6MM(D)	5,9	LOA001	LOCATOR ABUTMENT 4.1MM(D) X 1MM(H)	25
IWGA62C	CERTAIN UCLA GOLD (NON-HEXED) ABUTMENT CYLINDER 6MM(D)	9	LOA002	LOCATOR ABUTMENT 4.1MM(D) X 2MM(H)	25
IWGA62T	CERTAIN UCLA GOLD (NON-HEXED) ABUTMENT CYLINDER 6MM(D) W/LARGE DIAMETER TITANIUM SCREW	9	LOA003	LOCATOR ABUTMENT 4.1MM(D) X 3MM(H)	25
IWIP50	CERTAIN STRAIGHT PICK-UP COPING 5MM(D) X 5MM(P)	4,6,10	LOA004	LOCATOR ABUTMENT 4.1MM(D) X 4MM(H)	25
IWIP55	CERTAIN EP® PICK-UP COPING 5MM(D) X 5.6MM(P)	4,6,10	LOA005	LOCATOR ABUTMENT 4.1MM(D) X 5MM(H)	25
IWIP56	CERTAIN EP PICK-UP COPING 5MM(D) X 6MM(P)	4,6,10	LOA006	LOCATOR ABUTMENT 4.1MM(D) X 6MM(H)	25
IWIP60	CERTAIN STRAIGHT PICK-UP COPING 6MM(D) X 6MM(P)	4,6,10	LOAB	LOCATOR BAR ATTACHMENT	14,26
IWIP66	CERTAIN EP PICK-UP COPING 6MM(D) X 6.6MM(P)	4,6,10	LOAD	LOCATOR BAR ATTACHMENT DRILL	14,26
IWIT50	CERTAIN STRAIGHT TRANSFER COPING 5MM(D) X 5MM(P)	4,6,10	LOADT4	LOCATOR ABUTMENT DRIVER TIP 24MM(L)	14,26,30
IWIT55	CERTAIN EP TWIST LOCK™ COPING 5MM(D) X 5.6MM(P)	4,6,10	LOADT9	LOCATOR ABUTMENT DRIVER TIP 30MM(L)	14,26,30
IWIT56	CERTAIN EP TWIST LOCK COPING 5MM(D) X 6MM(P)	4,6,10	LOAH	LOCATOR REPLACEMENT HOUSING	14,26
IWIT60	CERTAIN STRAIGHT TRANSFER COPING 6MM(D) X 6MM(P)	4,6,10	LOAT	LOCATOR BAR ATTACHMENT TAP	14,26
IWIT66	CERTAIN EP TWIST LOCK COPING 6MM(D) X 6.6MM(P)	4,6,10	LORHK	LOCATOR REPLACEMENT HOUSING KIT	14,26
IWPC52C	CERTAIN UCLA CASTABLE (NON-HEXED) ABUTMENT CYLINDER 5MM(D)	9	LPAC3217	LOW PROFILE 17° PRE-ANGLED ABUTMENT 3.4MM(D) X 2MM(H)	23
IWPC52T	CERTAIN UCLA CASTABLE (NON-HEXED) ABUTMENT CYLINDER 5MM(D) 9 W/LARGE DIAMETER TITANIUM SCREW	9	LPAC3330	LOW PROFILE 30° PRE-ANGLED ABUTMENT 3.4MM(D) X 3MM(H)	23
IWPC62C	CERTAIN UCLA CASTABLE (NON-HEXED) ABUTMENT CYLINDER 6MM(D)	9	LPAC3417	LOW PROFILE 17° PRE-ANGLED ABUTMENT 3.4MM(D) X 4MM(H)	23
IWPC62T	CERTAIN UCLA CASTABLE (NON-HEXED) ABUTMENT CYLINDER 6MM(D) 9 W/LARGE DIAMETER TITANIUM SCREW	9	LPAC3530	LOW PROFILE 30° PRE-ANGLED ABUTMENT 3.4MM(D) X 5MM(H)	23
IWPPF554	CERTAIN PERFORMANCE POST 5MM(D) X 5MM(P) X 4MM(H)	1	LPAC4217	LOW PROFILE 17° PRE-ANGLED ABUTMENT 4.1MM(D) X 2MM(H)	23
IWPPF556	CERTAIN PERFORMANCE POST 5MM(D) X 5MM(P) X 6MM(H)	1	LPAC4330	LOW PROFILE 30° PRE-ANGLED ABUTMENT 4.1MM(D) X 3MM(H)	23
IWPPF664	CERTAIN PERFORMANCE POST 6MM(D) X 6MM(P) X 4MM(H)	1	LPAC4417	LOW PROFILE 17° PRE-ANGLED ABUTMENT 4.1MM(D) X 4MM(H)	23
IWPPF666	CERTAIN PERFORMANCE POST 6MM(D) X 6MM(P) X 6MM(H)	1	LPAC4530	LOW PROFILE 30° PRE-ANGLED ABUTMENT 4.1MM(D) X 5MM(H)	23
IWPFTC51	CERTAIN PERFORMANCE (HEXED) TEMPORARY CYLINDER 5MM(D)	2	LPAC5217	LOW PROFILE 17° PRE-ANGLED ABUTMENT 5MM(D) X 2MM(H)	23
			LPAC5330	LOW PROFILE 30° PRE-ANGLED ABUTMENT 5MM(D) X 3MM(H)	23
			LPAC5417	LOW PROFILE 17° PRE-ANGLED ABUTMENT 5MM(D) X 4MM(H)	23
			LPAC5530	LOW PROFILE 30° PRE-ANGLED ABUTMENT 5MM(D) X 5MM(H)	23

Index

Cat. #	Description	Page#	Cat. #	Description	Page#
LPC341	LOW PROFILE TWO-PIECE ABUTMENT 3.4MM(D) X 1MM(H)	23	MAP32G	GINGIHUE® POST 3.4MM(D) X 3.8MM(P) X 2MM(H)	17
LPC341U	LOW PROFILE ONE-PIECE ABUTMENT 3.4MM(D) X 1MM(H)	23	MAP34G	GINGIHUE POST 3.4MM(D) X 3.8MM(P) X 4MM(H)	17
LPC342	LOW PROFILE TWO-PIECE ABUTMENT 3.4MM(D) X 2MM(H)	23	MIC33	PICK-UP IMPRESSION COPING 3.4MM(D)	18,20,22
LPC342U	LOW PROFILE ONE-PIECE ABUTMENT 3.4MM(D) X 2MM(H)	23	MIDTH	MANUAL INTERCHANGEABLE DRIVER TIP HANDLE	30
LPC343	LOW PROFILE TWO-PIECE ABUTMENT 3.4MM(D) X 3MM(H)	23	MLOA001	LOCATOR® ABUTMENT 3.4MM(D) X 1MM(H)	25
LPC343U	LOW PROFILE ONE-PIECE ABUTMENT 3.4MM(D) X 3MM(H)	23	MLOA002	LOCATOR ABUTMENT 3.4MM(D) X 2MM(H)	25
LPC344	LOW PROFILE TWO-PIECE ABUTMENT 3.4MM(D) X 4MM(H)	23	MLOA003	LOCATOR ABUTMENT 3.4MM(D) X 3MM(H)	25
LPC344U	LOW PROFILE ONE-PIECE ABUTMENT 3.4MM(D) X 4MM(H)	23	MLOA004	LOCATOR ABUTMENT 3.4MM(D) X 4MM(H)	25
LPC441	LOW PROFILE TWO-PIECE ABUTMENT 4.1MM(D) X 1MM(H)	23	MLOA005	LOCATOR ABUTMENT 3.4MM(D) X 5MM(H)	25
LPC441U	LOW PROFILE ONE-PIECE ABUTMENT 4.1MM(D) X 1MM(H)	23	MLOA006	LOCATOR ABUTMENT 3.4MM(D) X 6MM(H)	25
LPC442	LOW PROFILE TWO-PIECE ABUTMENT 4.1MM(D) X 2MM(H)	23	MLT150	LAPPING TOOL FOR CASTABLE UCLA ABUTMENT W/GUIDE 3.4MM(D)	33
LPC442U	LOW PROFILE ONE-PIECE ABUTMENT 4.1MM(D) X 2MM(H)	23	MMILA	LAB ANALOG 3.4MM(D)	18,20,22
LPC443	LOW PROFILE TWO-PIECE ABUTMENT 4.1MM(D) X 3MM(H)	23	MMTCS1	TEMPORARY (HEXED) CYLINDER 3.4MM(D) W/RETENTION AND (HEXED) SCREW	16
LPC443U	LOW PROFILE ONE-PIECE ABUTMENT 4.1MM(D) X 3MM(H)	23	MPAP32G	GINGIHUE 15° PRE-ANGLED POST 3.4MM(D) X 3.8MM(P) X 2MM(H)	17
LPC444	LOW PROFILE TWO-PIECE ABUTMENT 4.1MM(D) X 4MM(H)	23	MPAP34G	GINGIHUE 15° PRE-ANGLED POST 3.4MM(D) X 3.8MM(P) X 4MM(H)	17
LPC444U	LOW PROFILE ONE-PIECE ABUTMENT 4.1MM(D) X 4MM(H)	23	MPAPF34	PREFORMANCE 15° PRE-ANGLED POST 3.4MM(D) X 3.8MM(P) X 4MM(H)	15
LPC541	LOW PROFILE TWO-PIECE ABUTMENT 5MM(D) X 1MM(H)	23	MPAPF36	PREFORMANCE 15° PRE-ANGLED POST 3.4MM(D) X 3.8MM(P) X 6MM(H)	15
LPC542	LOW PROFILE TWO-PIECE ABUTMENT 5MM(D) X 2MM(H)	23	MPFP34	PREFORMANCE POST 3.4MM(D) X 3.8MM(P) X 4MM(H)	15
LPC542U	LOW PROFILE ONE-PIECE ABUTMENT 5MM(D) X 2MM(H)	23	MPFP36	PREFORMANCE POST 3.4MM(D) X 3.8MM(P) X 6MM(H)	15
LPC543	LOW PROFILE TWO-PIECE ABUTMENT 5MM(D) X 3MM(H)	23	MPFTC32	PREFORMANCE (NON-HEXED) TEMPORARY CYLINDER 3.4MM(D)	16
LPC543U	LOW PROFILE ONE-PIECE ABUTMENT 5MM(D) X 3MM(H)	23	MPFTC34	PREFORMANCE (HEXED) TEMPORARY CYLINDER 3.4MM(D)	16
LPC544	LOW PROFILE TWO-PIECE ABUTMENT 5MM(D) X 4MM(H)	23	MSGIAM1	NAVIGATOR® CERTAIN® ANALOG MOUNT 3.4MM(D) X 1(L)	32
LPC544U	LOW PROFILE ONE-PIECE ABUTMENT 5MM(D) X 4MM(H)	23	MSGIAM2	NAVIGATOR CERTAIN ANALOG MOUNT 3.4MM(D) X 2(L)	32
LPCAMI	LOW PROFILE ABUTMENT LAPPING TOOL	12,24	MSGIAM3	NAVIGATOR CERTAIN ANALOG MOUNT 3.4MM(D) X 3(L)	32
LPGCC1	LOW PROFILE ABUTMENT (HEXED) CASTABLE CYLINDER	12,24	MSGIAM4	NAVIGATOR CERTAIN ANALOG MOUNT 3.4MM(D) X 4(L)	32
LPGCC2	LOW PROFILE ABUTMENT (NON-HEXED) CASTABLE CYLINDER	12,24	MUCC1C	UCLA CASTABLE (HEXED) ABUTMENT CYLINDER 3.4MM(D)	21
LPCDE	LOW PROFILE ABUTMENT DISTAL EXTENSION	12,24	MUCC2C	UCLA CASTABLE (NON-HEXED) ABUTMENT CYLINDER 3.4MM(D)	21
LPGGC1	LOW PROFILE ABUTMENT (HEXED) GOLD CYLINDER	12,24	MUCG1C	UCLA GOLD (HEXED) ABUTMENT CYLINDER 3.4MM(D)	19,21
LPGGC2	LOW PROFILE ABUTMENT (NON-HEXED) GOLD CYLINDER	12,24	MUCG2C	UCLA GOLD (NON-HEXED) ABUTMENT CYLINDER 3.4MM(D)	21
LPGGSH	LOW PROFILE ABUTMENT GOLD-TITE® RETAINING SCREW	12,24,27,28	MUNITS	SQUARE TRY-IN SCREW (5-PACK), 3.4MM(D)	18,20,22,28
LPCTSH	LOW PROFILE ABUTMENT TITANIUM RETAINING SCREW	12,24,27,28	NCATD0	CONTRA ANGLE TORQUE DRIVER KIT	29
LPCHC	LOW PROFILE ABUTMENT HEALING CAP	12,24	NCATD0C	CONTRA ANGLE TORQUE DRIVER KIT CERTAIN	29
LPCLA	LOW PROFILE ABUTMENT LAB ANALOG	12,24	NPSDK0	PROSTHETIC DRIVER KIT	29
LPCPIC1	LOW PROFILE ABUTMENT (HEXED) PICK-UP IMPRESSION COPING	12,24	PAA484	PROVIDE® ABUTMENT ANALOG 4.8MM(P) X 4MM(H)	8
LPCPIC2	LOW PROFILE ABUTMENT (NON-HEXED) PICK-UP IMPRESSION COPING	12,24	PAA485	PROVIDE ABUTMENT ANALOG 4.8MM(P) X 5.5MM(H)	8
LPCPP	LOW PROFILE ABUTMENT POLISHING PROTECTOR	12,24	PAA654	PROVIDE ABUTMENT ANALOG 6.5MM(P) X 4MM(H)	8
LPCPTC1	LOW PROFILE ABUTMENT (HEXED) PREFORMANCE® TEMPORARY CYLINDER	12,24	PAA655	PROVIDE ABUTMENT ANALOG 6.5MM(P) X 5.5MM(H)	8
LPCPTC2	LOW PROFILE ABUTMENT (NON-HEXED) PREFORMANCE TEMPORARY CYLINDER	12,24	PAAP48	PROVIDE ABUTMENT ANALOG WITH PIN 4.8MM(P)	8
LPCQB	LOW PROFILE ABUTMENT QUICKBRIDGE®	12,24	PAAP65	PROVIDE ABUTMENT ANALOG WITH PIN 6.5MM(P)	8
LPCQBCAP	LOW PROFILE ABUTMENT QUICKBRIDGE REPLACEMENT CAP	12,24	PAD00	POSTERIOR ABUTMENT DRIVER 17MM(L)	29,30
LPCRIC	LOW PROFILE ABUTMENT QUICKBRIDGE IMPRESSION COPING	12,24	PAD24	STANDARD ABUTMENT DRIVER 24MM(L)	29,30
LPCTC1	LOW PROFILE ABUTMENT (HEXED) TEMPORARY CYLINDER	12,24	PAK4140	PROVIDE ABUTMENT PLACEMENT KIT 4.1MM(D) X 4.8MM(P) X 1MM(H) - 4MM POST	7
LPCTC2	LOW PROFILE ABUTMENT (NON-HEXED) TEMPORARY CYLINDER	12,24	PAK4155	PROVIDE ABUTMENT PLACEMENT KIT 4.1MM(D) X 4.8MM(P) X 1MM(H) - 5.5MM POST	7
LPCTIC1	LOW PROFILE ABUTMENT (HEXED) TRANSFER IMPRESSION COPING	12,24	PAK4240	PROVIDE ABUTMENT PLACEMENT KIT 4.1MM(D) X 4.8MM(P) X 2MM(H) - 4MM POST	7
LPCTIC2	LOW PROFILE ABUTMENT (NON-HEXED) TRANSFER IMPRESSION COPING	12,24	PAK4255	PROVIDE ABUTMENT PLACEMENT KIT 4.1MM(D) X 4.8MM(P) X 2MM(H) - 5.5MM POST	7
LPCTSH	LOW PROFILE ABUTMENT TITANIUM RETAINING SCREW	12,24	PAK4340	PROVIDE ABUTMENT PLACEMENT KIT 4.1MM(D) X 4.8MM(P) X 3MM(H) - 4MM POST	7
LPCTUCA	LOW PROFILE ABUTMENT LASER WELDED CYLINDER	12,24	PAK4355	PROVIDE ABUTMENT PLACEMENT KIT 4.1MM(D) X 4.8MM(P) X 3MM(H) - 5.5MM POST	7
LPCWS	LOW PROFILE ABUTMENT WAXING SCREW	12,24			
LT150	LAPPING TOOL FOR CASTABLE UCLA ABUTMENT W/GUIDE 4MM(D)	33			
LTAH5	LABORATORY ABUTMENT HOLDER FOR 3.4MM(D)	18,20,22,33			
LTAH7	LABORATORY HOLDER FOR 4.1, 5, 6MM(D)	18,20,22,33			
L-TIRW	LOW TORQUE INDICATING RATCHET WRENCH	29,33			

Index

Cat. #	Description	Page#	Cat. #	Description	Page#
PAK4440	PROVIDE® ABUTMENT PLACEMENT KIT 4.1MM(D) X 4.8MM(P) X 4MM(H) - 4MM POST	7	PHD02N	NARROW POSTERIOR LARGE HEX DRIVER 17MM(L)	27,28,29,30
PAK4455	PROVIDE ABUTMENT PLACEMENT KIT 4.1MM(D) X 4.8MM(P) X 4MM(H) - 5.5MM POST	7	PHD03N	NARROW STANDARD LARGE HEX DRIVER 24MM(L)	27,28,29,30
PAK5140	PROVIDE ABUTMENT PLACEMENT KIT 5MM(D) X 6.5MM(P) X 1MM(H) - 4MM POST	7	PIC484	PROVIDE IMPRESSION COPING 4.8MM(P) X 4MM(H)	8
PAK5155	PROVIDE ABUTMENT PLACEMENT KIT 5MM(D) X 6.5MM(P) X 1MM(H) - 5.5MM POST	7	PIC484H	PROVIDE IMPRESSION COPING WITH HOLES 4.8MM(P) X 4MM(H)	8
PAK5240	PROVIDE ABUTMENT PLACEMENT KIT 5MM(D) X 6.5MM(P) X 2MM(H) - 4MM POST	7	PIC485	PROVIDE IMPRESSION COPING 4.8MM(P) X 5.5MM(H)	8
PAK5255	PROVIDE ABUTMENT PLACEMENT KIT 5MM(D) X 6.5MM(P) X 2MM(H) - 5.5MM POST	7	PIC485H	PROVIDE IMPRESSION COPING WITH HOLES 4.8MM(P) X 5.5MM(H)	8
PAK5340	PROVIDE ABUTMENT PLACEMENT KIT 5MM(D) X 4.8MM(P) X 3MM(H) - 4MM POST	7	PIC654	PROVIDE IMPRESSION COPING 6.5MM(P) X 4MM(H)	8
PAK5355	PROVIDE ABUTMENT PLACEMENT KIT 5MM(D) X 6.5MM(P) X 3MM(H) - 5.5MM POST	7	PIC654H	PROVIDE IMPRESSION COPING WITH HOLES 6.5MM(P) X 4MM(H)	8
PAK5440	PROVIDE ABUTMENT PLACEMENT KIT 5MM(D) X 4.8MM(P) X 4MM(H) - 4MM POST	7	PIC655	PROVIDE IMPRESSION COPING 6.5MM(P) X 5.5MM(H)	8
PAK5455	PROVIDE ABUTMENT PLACEMENT KIT 5MM(D) X 4.8MM(P) X 4MM(H) - 5.5MM POST	7	PIC655H	PROVIDE IMPRESSION COPING WITH HOLES 6.5MM(P) X 5.5MM(H)	8
PAK6140	PROVIDE ABUTMENT PLACEMENT KIT 6MM(D) X 6.5MM(P) X 1MM(H) - 4MM POST	7	PPC484	PROVIDE PROTECTION CAP 4.8MM(P) X 4MM(H)	8
PAK6155	PROVIDE ABUTMENT PLACEMENT KIT 6MM(D) X 6.5MM(P) X 1MM(H) - 5.5MM POST	7	PPC485	PROVIDE PROTECTION CAP 4.8MM(P) X 5.5MM(H)	8
PAK6240	PROVIDE ABUTMENT PLACEMENT KIT 6MM(D) X 6.5MM(P) X 2MM(H) - 4MM POST	7	PPC654	PROVIDE PROTECTION CAP 6.5MM(P) X 4MM(H)	8
PAK6255	PROVIDE ABUTMENT PLACEMENT KIT 6MM(D) X 6.5MM(P) X 2MM(H) - 5.5MM POST	7	PPC655	PROVIDE PROTECTION CAP 6.5MM(P) X 5.5MM(H)	8
PAK6340	PROVIDE ABUTMENT PLACEMENT KIT 6MM(D) X 6.5MM(P) X 3MM(H) - 4MM POST	7	PPIA3	POLISHING PROTECTOR UCLA ABUTMENT 4.1MM(D)	33
PAK6355	PROVIDE ABUTMENT PLACEMENT KIT 6MM(D) X 6.5MM(P) X 3MM(H) - 5.5MM POST	7	PPMM1	POLISHING PROTECTOR UCLA 3.4MM(D)	33
PAK6440	PROVIDE ABUTMENT PLACEMENT KIT 6MM(D) X 6.5MM(P) X 4MM(H) - 4MM POST	7	PRK484	PROVIDE ABUTMENT RESTORATIVE KIT 4.8MM(P) - 4MM POST	7
PAK6455	PROVIDE ABUTMENT PLACEMENT KIT 6MM(D) X 6.5MM(P) X 4MM(H) - 5.5MM POST	7	PRK485	PROVIDE ABUTMENT RESTORATIVE KIT 4.8MM(P) - 5.5MM POST	7
PAP452G	GINGIHUE® 15° PRE-ANGLED POST 4.1MM(D) X 5MM(P) X 2MM(H)	17	PRK654	PROVIDE ABUTMENT RESTORATIVE KIT 6.5MM(P) - 4MM POST	7
PAP454G	GINGIHUE 15° PRE-ANGLED POST 4.1MM(D) X 5MM(P) X 4MM(H)	17	PRK655	PROVIDE ABUTMENT RESTORATIVE KIT 6.5MM(P) - 5.5MM POST	7
PAP462G	GINGIHUE 15° PRE-ANGLED POST 4.1MM(D) X 6MM(P) X 2MM(H)	17	PSD00	POSTERIOR SLOTTED SCREW DRIVER - SLOTTED 17MM(L)	29
PAP464G	GINGIHUE 15° PRE-ANGLED POST 4.1MM(D) X 6MM(P) X 4MM(H)	17	PSD01	STANDARD SLOTTED SCREW DRIVER - SLOTTED 24MM(L)	29
PAP552G	GINGIHUE 15° PRE-ANGLED POST 5MM(D) X 5MM(P) X 2MM(H)	17	PSDT1	PROSTHETIC SYSTEM DRIVER TRAY	29
PAP554G	GINGIHUE 15° PRE-ANGLED POST 5MM(D) X 5MM(P) X 4MM(H)	17	PSQD0N	NARROW POSTERIOR SQUARE DRIVER 17MM(L)	28,29,30
PAP562G	GINGIHUE 15° PRE-ANGLED POST 5MM(D) X 6MM(P) X 2MM(H)	17	PSQD1N	NARROW STANDARD SLOTTED SQUARE DRIVER 24MM(L)	28,29,30
PAP564G	GINGIHUE 15° PRE-ANGLED POST 5MM(D) X 6MM(P) X 4MM(H)	17	PUA48M	PROVIDE TEMPORARY CYLINDER MULTI-UNIT - 4.8MM PROFILE	8
PAP662G	GINGIHUE 15° PRE-ANGLED POST 6MM(D) X 6MM(P) X 2MM(H)	17	PUA48S	PROVIDE TEMPORARY CYLINDER SINGLE-UNIT - 4.8MM PROFILE	8
PAP664G	GINGIHUE 15° PRE-ANGLED POST 6MM(D) X 6MM(P) X 4MM(H)	17	PUA65M	PROVIDE TEMPORARY CYLINDER MULTI-UNIT - 6.5MM PROFILE	8
PAPF454	PREFORMANCE® 15° PRE-ANGLED POST 4.1MM(D) X 5MM(P) X 4MM(H)	15	PUA65S	PROVIDE TEMPORARY CYLINDER SINGLE-UNIT - 6.5MM PROFILE	8
PAPF456	PREFORMANCE 15° PRE-ANGLED POST 4.1MM(D) X 5MM(P) X 6MM(H)	15	PWS48M	PROVIDE WAXING SLEEVE 4.8MM(P) MULTI-UNIT	8
PAPF554	PREFORMANCE 15° PRE-ANGLED POST 5MM(D) X 5MM(P) X 4MM(H)	15	PWS48S	PROVIDE WAXING SLEEVE 4.8MM(P) SINGLE-UNIT	8
PAPF556	PREFORMANCE 15° PRE-ANGLED POST 5MM(D) X 5MM(P) X 6MM(H)	15	PWS65M	PROVIDE WAXING SLEEVE 6.5MM(P) MULTI-UNIT	8
PAPF664	PREFORMANCE 15° PRE-ANGLED POST 6MM(D) X 6MM(P) X 4MM(H)	15	PWS65S	PROVIDE WAXING SLEEVE 6.5MM(P) SINGLE-UNIT	8
PAPF666	PREFORMANCE 15° PRE-ANGLED POST 6MM(D) X 6MM(P) X 6MM(H)	15	RASA3	RIGHT ANGLE ABUTMENT DRIVER TIP - STEEL	29,30
PEMODLOC	PATIENT ED MODEL - LOCATOR®	34	RASD1	RIGHT ANGLE SLOTTED DRIVER TIP 24MM(L)	29
PEMODSM	PATIENT ED MODEL - SINGLE/MULTIPLE TEETH	34	RASD6	RIGHT ANGLE SLOTTED DRIVER TIP 30MM(L)	29
PFP454	PREFORMANCE POST 4.1MM(D) X 5MM(P) X 4MM(H)	15	RASH2N	NARROW RIGHT ANGLE SMALL (HEXED) DRIVER TIP 24MM(L)	30
PFP456	PREFORMANCE POST 4.1MM(D) X 5MM(P) X 6MM(H)	15	RASH3N	NARROW RIGHT ANGLE LARGE (HEXED) DRIVER TIP 24MM(L)	27,28,29,30
PFTC41	PREFORMANCE (HEXED) TEMPORARY CYLINDER 4.1MM(D)	16	RASH4	RIGHT ANGLE DRIVER TIP 50 IN. (HEXED) 24MM(L)	14,26,30
PFTC42	PREFORMANCE (NON-HEXED) TEMPORARY CYLINDER 4.1MM(D)	16	RASH7N	NARROW RIGHT ANGLE SMALL (HEXED) DRIVER TIP 30MM(L)	30
PHD00N	NARROW POSTERIOR SMALL HEX DRIVER 17MM(L)	30	RASH8N	NARROW RIGHT ANGLE LARGE (HEXED) DRIVER TIP 30MM(L)	27,28,29,30
PHD01N	NARROW STANDARD SMALL HEX DRIVER 24MM(L)	30	RASH9	RIGHT ANGLE DRIVER TIP 50 IN. (HEXED) 30MM(L)	14,26,30
			RASQ3N	NARROW RIGHT ANGLE SQUARE DRIVER TIP 24MM(L)	28,29,30
			RASQ8N	NARROW RIGHT ANGLE SQUARE DRIVER TIP 30MM(L)	28,29,30
			RH600	REAMER/HANDLE FOR SGC34, UNAB1/2	33
			RTI2035TR	RESTORATIVE TORQUE INDICATOR TRAY	29
			SGIAM41	NAVIGATOR® CERTAIN® ANALOG MOUNT 4.1MM(D) X 1(L)	32
			SGIAM42	NAVIGATOR CERTAIN ANALOG MOUNT 4.1MM(D) X 2(L)	32
			SGIAM43	NAVIGATOR CERTAIN ANALOG MOUNT 4.1MM(D) X 3(L)	32
			SGIAM44	NAVIGATOR CERTAIN ANALOG MOUNT 4.1MM(D) X 4(L)	32
			SGIAM51	NAVIGATOR CERTAIN ANALOG MOUNT 5MM(D) X 1(L)	32
			SGIAM52	NAVIGATOR CERTAIN ANALOG MOUNT 5MM(D) X 2(L)	32
			SGIAM53	NAVIGATOR CERTAIN ANALOG MOUNT 5MM(D) X 3(L)	32
			SGIAM54	NAVIGATOR CERTAIN ANALOG MOUNT 5MM(D) X 4(L)	32
			SGLKIT	NAVIGATOR LABORATORY KIT	32

Index

Cat. #	Description	Page#	Cat. #	Description	Page#
SGLTRAY	NAVIGATOR® LABORATORY TRAY	32	WPP664G	GINGIHUE POST 6MM(D) X 6MM(P) X 4MM(H)	17
SGUCA1C	UCLA GOLD STANDARD ZR (HEXED) ABUTMENT CYLINDER 4.1MM(D)	19,21	WSK10	ABUTMENT WAXING SCREW/GUIDE PIN-KNURLED 10MM(L)	28
SRT01	HAND TAP FOR SRT10	33	WSK15	ABUTMENT WAXING SCREW/GUIDE PIN-KNURLED 15MM(L)	28
SRT02	HAND DRILL 14MM(D) BRONZE DRILL FOR SRT10	33	WSK30	ABUTMENT WAXING SCREW/GUIDE PIN-KNURLED 20MM(L)	28
SRT03	HAND DRILL 1.18MM(D) SILVER DRILL FOR SRT10	33	WSU30	LABORATORY WAXING SCREW/GUIDE PIN-KNURLED	28
SRT04	EXTRACTING DRILL - ISO LATCH FOR SRT10	33	WTCS51	TEMPORARY (HEXED) IMPLANT CYLINDER 5MM(D)	16
SRT05	GUIDE HANDLE FOR SRT10	33	WTCS52	TEMPORARY (NON-HEXED) IMPLANT CYLINDER 5MM(D)	16
SRT10	SCREW REMOVING KIT	33	WTCS61	TEMPORARY (HEXED) IMPLANT CYLINDER 6MM(D)	16
SWG51C	UCLA GOLD STANDARD ZR (HEXED) ABUTMENT CYLINDER 5MM(D)	19,21	WTCS62	TEMPORARY (NON-HEXED) IMPLANT CYLINDER 6MM(D)	16
SWG61C	UCLA GOLD STANDARD ZR (HEXED) ABUTMENT CYLINDER 6MM(D)	19,21			
TD-10	CONTRA ANGLE TORQUE CONTROLLER 10NCM	29			
TD-20	CONTRA ANGLE TORQUE CONTROLLER 20NCM	29			
TD-35	CONTRA ANGLE TORQUE CONTROLLER 32NCM	29			
THRC4	TEMPORARY HEALING RETENTION CYLINDER 4.1MM(D) X 4MM(H)	25			
THRC6	TEMPORARY HEALING RETENTION CYLINDER 4.1MM(D) X 6MM(H)	25			
TMP80	TISSUE MEASURING POST	33			
UNA125	UCLA CASTABLE (HEXED) ABUTMENT CYLINDER (25-PACK)	19,21			
UNA225	UCLA CASTABLE (NON-HEXED) ABUTMENT CYLINDER (25-PACK)	21			
UNAB1C	UCLA CASTABLE (HEXED) ABUTMENT CYLINDER	19,21			
UNAB2C	UCLA CASTABLE (NON-HEXED) ABUTMENT CYLINDER	21			
UNIHG	GOLD-TITE® (HEXED) SCREW	18,20,22,28			
UNIHT	TITANIUM (HEXED) SCREW	18,20,22,28			
UNISG	GOLD-TITE SQUARE SCREW	18,20,22,28			
UNITS	SQUARE TRY-IN SCREW (5-PACK) 4.1, 5, 6MM(D)	18,20,22,28			
WCAP564	ZIREAL® POST 5MM(D) X 6MM(P) X 4MM(H)	17			
WGA51C	UCLA GOLD (HEXED) ABUTMENT CYLINDER 5MM(D)	19,21			
WGA52C	UCLA GOLD (NON-HEXED) ABUTMENT CYLINDER 5MM(D)	21			
WGA61C	UCLA GOLD (HEXED) ABUTMENT CYLINDER 6MM(D)	19,21			
WGA62C	UCLA GOLD (NON-HEXED) ABUTMENT CYLINDER 6MM(D)	21			
WIP55	IMPLANT EP® PICK-UP COPING 5MM(D) X 5MM(P)	18,20,22			
WIP56	IMPLANT EP PICK-UP COPING 5MM(D) X 6MM(P)	18,20,22			
WIP66	IMPLANT EP PICK-UP COPING 6MM(D) X 6MM(P)	18,20,22			
WIT55	IMPLANT EP TWIST LOCK™ COPING 5MM(D) X 5MM(P)	18,20,22			
WIT56	IMPLANT EP TWIST LOCK COPING 5MM(D) X 6MM(P)	18,20,22			
WIT66	IMPLANT EP TWIST LOCK COPING 6MM(D) X 6MM(P)	18,20,22			
WLT10	LAPPING TOOL FOR WIDE DIAMETER IMPLANTS	33			
WPC51C	UCLA CASTABLE (HEXED) ABUTMENT CYLINDER 5MM(D)	19,21			
WPC52C	UCLA CASTABLE (NON-HEXED) ABUTMENT CYLINDER 5MM(D)	21			
WPC61C	UCLA CASTABLE (HEXED) ABUTMENT CYLINDER 6MM(D)	19,21			
WPC62C	UCLA CASTABLE (NON-HEXED) ABUTMENT CYLINDER 6MM(D)	21			
WPP554	PREFORMANCE® POST 5MM(D) X 5MM(P) X 4MM(H)	15			
WPP556	PREFORMANCE POST 5MM(D) X 5MM(P) X 6MM(H)	15			
WPP664	PREFORMANCE POST 6MM(D) X 6MM(P) X 4MM(H)	15			
WPP666	PREFORMANCE POST 6MM(D) X 6MM(P) X 6MM(H)	15			
WPFTC51	PREFORMANCE (HEXED) TEMPORARY CYLINDER 5MM	16			
WPFTC52	PREFORMANCE (NON-HEXED) TEMPORARY CYLINDER 5MM	16			
WPFTC61	PREFORMANCE (HEXED) TEMPORARY CYLINDER 6MM	16			
WPFTC62	PREFORMANCE (NON-HEXED) TEMPORARY CYLINDER 6MM	16			
WPP50	POLISHING PROTECTOR 5MM(D)	33			
WPP552G	GINGIHUE® POST 5MM(D) X 5MM(P) X 2MM(H)	17			
WPP554G	GINGIHUE POST 5MM(D) X 5MM(P) X 4MM(H)	17			
WPP562G	GINGIHUE POST 5MM(D) X 6MM(P) X 2MM(H)	17			
WPP564G	GINGIHUE POST 5MM(D) X 6MM(P) X 4MM(H)	17			
WPP60	POLISHING PROTECTOR 6MM(D)	33			
WPP662G	GINGIHUE POST 6MM(D) X 6MM(P) X 2MM(H)	17			

Ordering Form

Customer Account#

Date: ____/____/____
Representative taking order

Customer Name: _____ Specialty: _____

Bill To: _____

Customer P.O. #: _____

Phone #: () _____

Method of Shipment: ____ FedEx ____ UPS

Ship To: _____

- Next Day by 8:30am
 Next Day by 10:30am
 Next Day - Afternoon
 Two Day
 Ground
 Other _____

Phone #: () _____

Would you like to receive information via email about BIOMET **3i**'s Products, Services and Events?

Yes No

Email Address: _____

Method of Payment:

Credit Card: ____ Visa ____ MasterCard ____ AMEX
 Card #: _____
 Expiration Date: _____

Special Instructions:

C.O.D.

Contact Name:

Bill - Net 30

Product No.	Quantity	Description	Discount	Unit Price	Total

Date:	Order Number:	Order Total:	Customer Service Representative:
-------	---------------	--------------	----------------------------------

Ordering Information

Some products may not be available outside the U.S.A.
Algunos productos no se comercializan fuera de EE.UU.
Certains produits ne sont pas disponibles en dehors des États-Unis.
Einige Produkte sind außerhalb der USA nicht erhältlich.

To Place an Order:

Contact your local BIOMET **3i** Representative or call:

BIOMET **3i** Customer Service
Monday–Thursday 8am–8pm (EST)
Friday 8am–6:30pm (EST)
800-342-5454, Fax 561-776-1272
In Canada: 800-363-1980, Outside US: 561-776-6700

TERMS AND CONDITIONS OF SALE. The following are the terms and conditions by which BIOMET **3i** sells its products.

GOVERNING TERMS. Any shipment of products shall be deemed to be on the terms and conditions stated herein. Any and all terms and conditions submitted by Purchaser are hereby rejected.

TAXES. The prices set forth herein do not include any sales, use, excise, ad valorem, property or other taxes applicable to the sale, use or delivery of the products, all of which shall be paid by Purchaser separately or added to the contract price and paid by Purchaser to BIOMET **3i**.

PRICES. The prices set forth for the products are in United States Dollars.

DELIVERY. Products sold hereunder shall be delivered by BIOMET **3i**, F.O.B. Palm Beach Gardens, Florida.

PAYMENT. Payment terms shall be as set forth under the Terms section on front of the invoice.

WARRANTY. BIOMET **3i** nor any of its affiliates make any warranty, express or implied, except that its products shall be free from defects in material and/or workmanship. This warranty applies only to the original Purchaser. In the event of a product defect, immediately notify BIOMET **3i** of the defect prior to returning the product. Devices shall be sterilized prior to return. As its sole obligation and as Purchaser's sole remedy under this warranty, BIOMET **3i** will, at its option, either repair, replace or issue credit for such products. Purchaser assumes all risks and liability resulting from the use of these products, whether used separately or in combination with other products.

Except for the warranty expressly described in the warranty paragraph above, neither BIOMET **3i** nor any of its affiliates makes any other warranty with respect to the BIOMET **3i** Products, expressed or implied, written or oral, including, without limitation, any implied warranty of merchantability, or a warranty of fitness for a particular purpose.

EDUCATION; MODIFICATION OF PRODUCTS. BIOMET **3i** reserves the right to modify products, discontinue products and change specifications of products.

RETURN POLICY. A Purchaser may return any BIOMET **3i** Product within 90 days of the invoice date. BIOMET **3i** Products returned within 60 days of the invoice date will be accepted without any re-stocking fee to the Purchaser. BIOMET **3i** Products returned between 61 and 90 days of the invoice date will be subject to a 15% restocking fee. A BIOMET **3i** Product will be accepted for return only if the BIOMET **3i** Product is (1) returned in its original, unopened package (including autoclavable products); (2) received by BIOMET **3i** within 90 days after the invoice date for that product; and (3) returned freight prepaid to 4555 Riverside Drive, Palm Beach Gardens, Florida 33410, (Attention: Returns Department) accompanied by the BIOMET **3i** Return Authorization Number provided by the BIOMET **3i** Customer Service Department. Purchaser should be advised that BIOMET **3i** Products not meeting the above criteria will not be accepted for return.

EXCHANGE POLICY. BIOMET **3i** Products may be exchanged within 180 days of the invoice date, without a re-stocking fee, for other BIOMET **3i** Products of equal or lesser value within the same product family as determined by BIOMET **3i** (ex. implant for implant, abutment for abutment, membrane for membrane). BIOMET **3i** Products may be exchanged within 180 days of the invoice date for other BIOMET **3i** Products of greater value within the same product family as determined by BIOMET **3i** (ex. implant for implant, abutment for abutment, membrane for membrane), with the price differential paid by the Purchaser. In both cases, the exchanged BIOMET **3i** Product must be (1) returned in its original, unopened package (including autoclavable products); (2) a currently offered BIOMET **3i** Product (discontinued product not included); and (3) returned freight prepaid to 4555 Riverside Drive, Palm Beach Gardens, Florida 33410, (Attention: Returns Department) and accompanied by the BIOMET **3i** Products Return Authorization Number provided by the BIOMET **3i** Customer Service Department.

AVAILABILITY OF PRODUCTS. All products not available in all areas. Any offer or product void where prohibited by law.

EXPORT CONTROL. All products are subject to all applicable export control and sanctions legislation.

FORCE MAJEURE. BIOMET **3i** shall not be liable for any loss or damage due to failure or delay arising out of any cause beyond the reasonable control of BIOMET **3i**. In the event of any failure or delay resulting from such causes, an equitable adjustment of delivery and any other appropriate terms and conditions shall be made. No such failure or delay shall be the basis for an increase of obligation by BIOMET **3i** nor any termination by the Purchaser.

LIMITATION OF LIABILITY. Under no circumstances shall BIOMET **3i** nor any of its affiliates be liable for business interruption, loss of profits, special, indirect, incidental or consequential damages of any nature and from any cause whether based in contract, warranty or tort (including negligence) or other legal theory, even if BIOMET **3i** has been advised of the possibility of such damages.

VALIDITY. If any provision of these Terms and Conditions is found to be illegal or unenforceable in any respect, such illegality or unenforceability shall not affect any other provision of these Terms and Conditions, all of which shall remain enforceable in accordance with their terms.

GENERAL PROVISIONS. The purchase of the products and these Terms and Conditions are governed by the laws of Florida without regard to conflicts of law principles. This document incorporates all oral and written representations between the parties and constitutes the entire agreement and understanding of the parties with respect to the subject matter hereof and supercedes any and all other agreements either oral or written between the parties with respect to such subject matter. No amendment or modification may be made to this document unless made in writing and duly executed by an authorized representative of BIOMET **3i**.

CAUTION. Federal (U.S.) Law restricts these devices to sale by or on the order of a licensed healthcare practitioner. Devices labeled STERILE are certified to be sterile unless sterile package is opened or damaged.

EXPORT ORDERS. Require advance payment or letter of credit. Shipments are made either by freight collect or paid by BIOMET **3i** and added to the invoice. Unless special instructions are received with an order, the shipping method will be determined by BIOMET **3i**, F.O.B. Palm Beach Gardens, Florida.

DUNS #: 186127825
BIOMET **3i** is listed in the SAM (U.S. System for Award Management) Database.
©2013 BIOMET **3i** LLC.



Want More? Solutions Start Here

VISIT
www.biomet3i.com

For More Information, Please Contact Your Local BIOMET 3i Sales Representative

BIOMET 3i™



BIOMET 3i
4555 Riverside Drive
Palm Beach Gardens, FL 33410
1-800-342-5454
Outside The U.S.: +1-561-776-6700
Fax: +1-561-776-1272
www.biomet3i.com

EC REP BIOMET 3i
Dental Iberica S.L.
WTC Almeda Park, Ed. 1, Planta 1ª
Pl. de la Pau, s/n
08940, Cornellà de Llobregat
(Barcelona) Spain
Phone: +34-93-470-55-00
Fax: +34-93-371-78-49



Join
Us



Follow
Us



Watch
Us



Download
It

All trademarks herein are the property of BIOMET 3i LLC unless otherwise indicated. This material is intended for laboratories and clinicians only and is not intended for patient distribution. This material is not to be redistributed, duplicated, or disclosed without the express written consent of BIOMET 3i. For additional product information, including indications, contraindications, warnings, precautions, and potential adverse effects, see the product package insert and the BIOMET 3i Website.

3i T3, BellaTek, BellaTek design, Certain, DIEM, Encode, EP, GingiHue, Gold-Tite, IOL, Navigator, OSSEOTITE, PreFormance, PREVAL, Provide, QuickBridge, QuickSeat and ZiReal are registered trademarks of BIOMET 3i LLC. NanoTite, Providing Solutions – One Patient At A Time and Twist Lock are trademarks of BIOMET 3i LLC. Dolder is a registered trademark of Prof. Eugen Dolder, formerly the director of School of Dentistry at the University in Zurich. LOCATOR is a registered trademark of Zest Anchors, Inc. ©2013 BIOMET 3i LLC.



CATRES
REV D 10/13